Cavitation Pro-1 Super Power Digital Skin Care Machine (SKU16628)



SKIN+ACT

Toll Free: 1.800.418.0830	www.skinact.com www.spaandequipment.com	International: 818.834.6640

Copyright © 2026 Spa and Equipment, All Rights Reserved

NOTICE

No part of this document may be photocopied, reproduced, or translated into any other language without prior written consent of Spa and Equipment/SkinAct.

The information in this document is subject to change without notice at any time and should not be construed as a commitment by Spa and Equipment/SkinAct.

Spa and Equipment/SkinAct assumes no responsibility for any errors that may be in this document, nor does it make expressed or implied warranty with regard to this material, including, but not limited to, the implied warranties of merchantability and fitness for a particular purpose.

Spa and Equipment/SkinAct shall not be liable for incidental or consequential damages arising out of the furnishing, performance, or use of this document and the program material which it describes.

SKIN+ACT

Safety Notice

⚠ Before operation, please read the following carefully:

It is essential to select the appropriate program according to the specific treatment.

During use of this device, if you feel pain, discomfort, excessive heat, redness, or if marks appear on the skin, stop the operation immediately.

Do not use this device if you suffer from fever, inflammation, dermatitis (including acne, eczema, herpes), open wounds, or if you have serious or progressive illnesses such as cancer, AIDS, hepatitis, blood diseases, or blood coagulation disorders.

Do not apply this device if you have or have had phlebitis, have undergone vein surgery within the past two months, experience varicose veins, or tingling sensations in the limbs. If you have any concerns, please consult your physician before use.

This device must not be used on pregnant women.

Do not use this device if you suffer from epilepsy or any mental illness.

If you are undergoing long-term drug treatment (such as anti-inflammatory drugs, anticoagulants, or antibiotics), or if your skin bruises easily even with minor impact, please consult your physician before use.

Failure to follow the operating instructions may result in reduced effectiveness. If symptoms do not improve or if you have any doubts during use, consult a doctor. Results may vary depending on age, lifestyle, physical condition, and habits.

Persons with implanted metal stents or medical electronic devices are not permitted to use this machine.

Persons suffering from osteoporosis are not permitted to use this machine.

This machine may be used after plastic surgery only under the guidance and approval of a surgeon.

A conductive gel must be applied to the treatment area before use.

This machine is designed for professional use only.

Please pay attention to the following precautions before using this device:

1. Do not use the device over ribs or bony areas.

2. Do not use cavitation for more than 10 minutes per area per session.

3. People with known allergies or sensitive skin should not use this device.

4. People who bruise easily should not use this device.

Remarks

• The large body probe is suitable for larger treatment areas and for users with higher body fat.

• The smaller probe is suitable for slimmer users and for areas where the larger probe is not convenient, such as the arms.

Working Theory

1. What is cavitation?

Cavitation is a technology that uses ultrasonic waves to create micro-vibrations in the treated area. These vibrations may help improve the appearance of the skin and support body-contouring treatments when used correctly.

2. What is the function?


This device is designed to support:

• Body shaping / contouring

• Improving the appearance of cellulite-prone areas


• Helping promote a smoother-looking skin surface


When used properly, the treatment is generally comfortable; however, sensitivity varies by person.

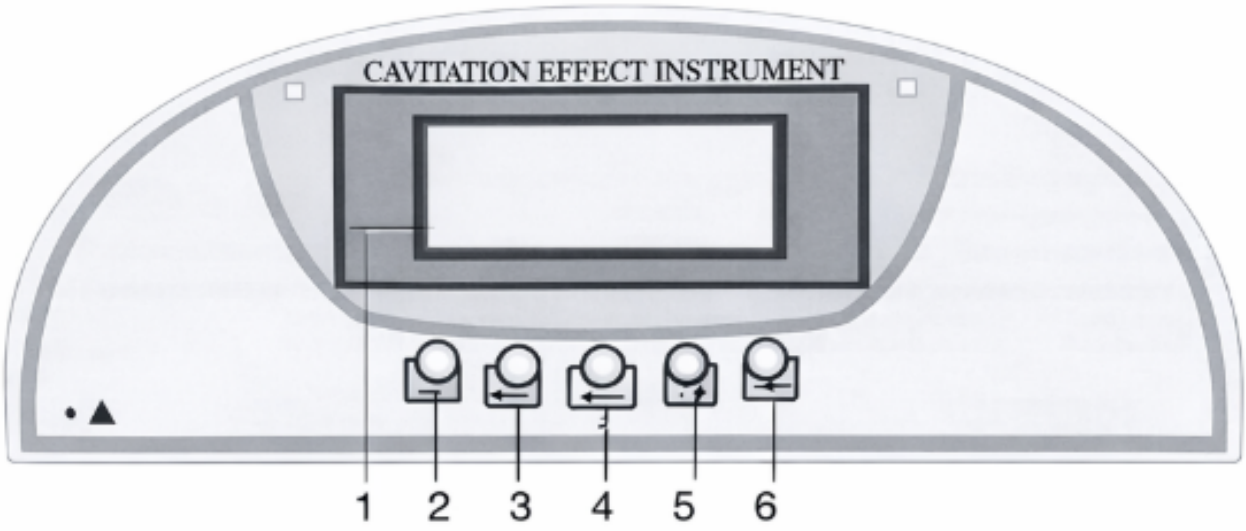

⚠ Notice: press the button power for 5seconds (less than 5seconds turn on the machine) then you can adjust the frequency

1° Display Screen
2° Menu select
3° Start/stop
4° Power switch
5° Parameter adjust " + "
6° Parameter adjust " - "

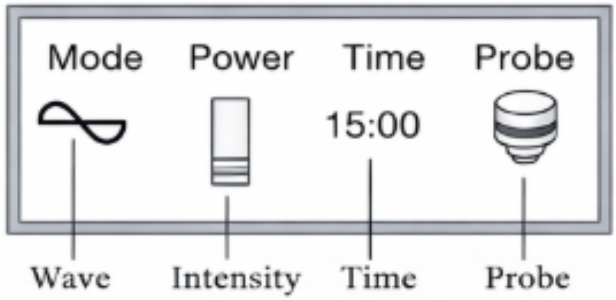

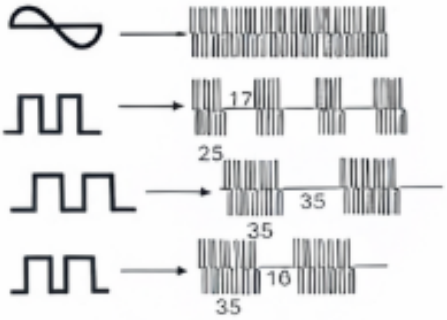



Note: The working frequency is 40KHz.



Cavitation Modes

Mode 1 – Continuous (∞): Constant output. Strongest fat reduction. Best for abdomen, thighs, buttocks.

Mode 2 – Pulse 1s ON / 1s OFF: Gentle and comfortable. Good for arms and sensitive clients.

Mode 3 – Pulse 2s ON / 2s OFF: Balanced strength. Good default mode for most treatments.

Mode 4 – Alternating Pulse: Skin tightening and toning. For maintenance, not heavy fat removal.

Treatment Frequency

2–3 sessions per week maximum. Leave 48–72 hours between sessions.

Client Aftercare


1. Drink at least 2 liters of water
2. Light exercise helps fat metabolism
3. Avoid alcohol and greasy foods for 24–48 hrs
4. Mild warmth or redness is normal

Operation


1. Connect the machine to the power supply and turn on the power.

2. Press the power button, and the machine will begin to operate (refer to the panel).


3. Select the desired wave mode by pressing the menu select button.
When the mode icon appears, press the parameter setting button to choose among the three wave modes.

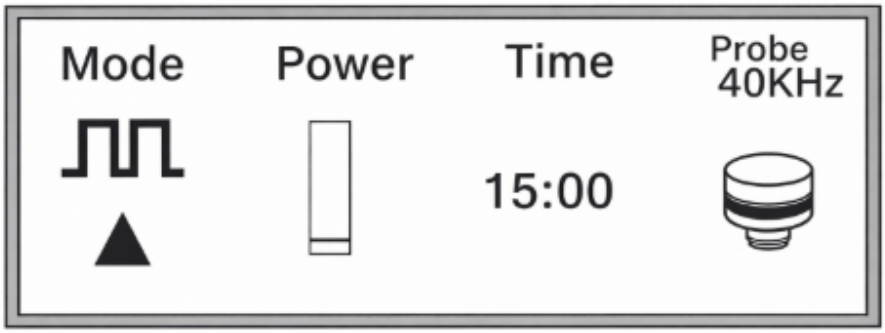

4. Press the menu select button again to choose the intensity. When the intensity icon appears, adjust the intensity by pressing the parameter adjustment buttons (refer to the panel).

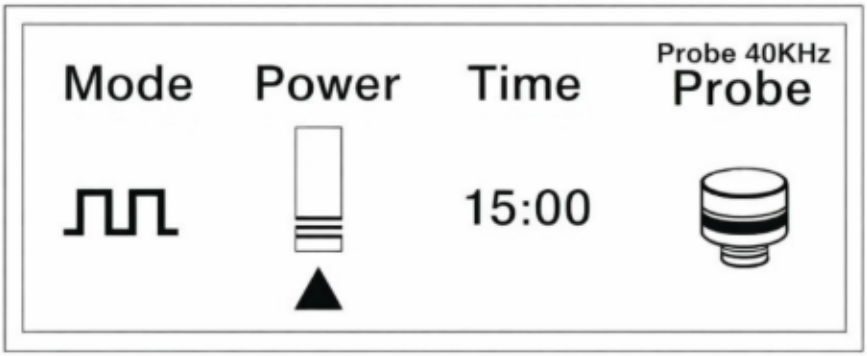


5. Adjust the time following steps 3 and 4.

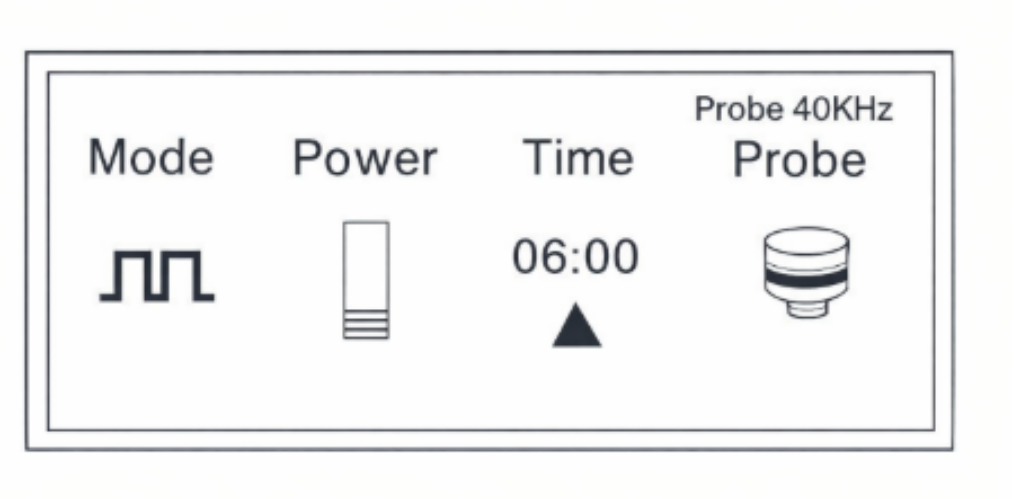

6. To switch probes, refer to steps 3 and 4.

Note: Stop the working probe before switching to another probe.

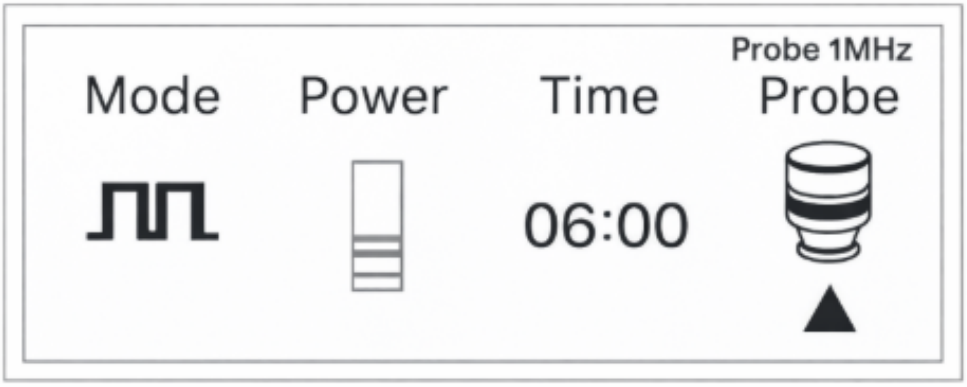


7. After completing the settings, press the start/stop button to begin operation.

Cavitation Treatment

Function: Slim Waist

1. Massage the abdomen for several minutes, then apply gel to the treatment area.

2. Set the parameters:

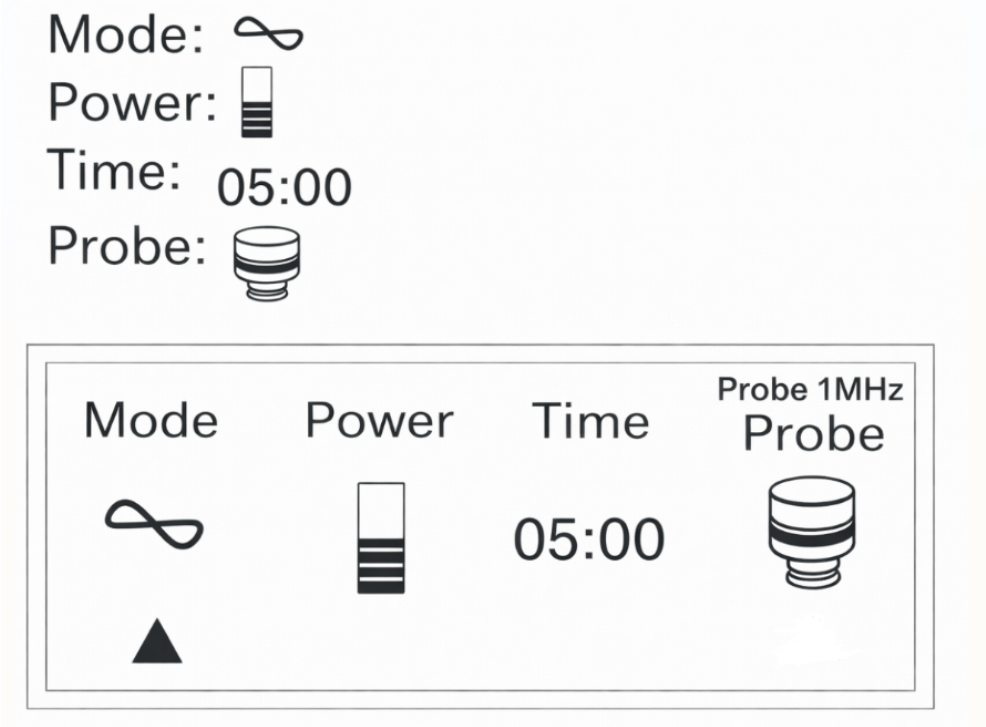

3. Operation method:


• Pinch the excess fat with one hand, hold the probe with the other hand, and move the probe from top to bottom or left to right over the fat.
• Avoid the ribs during operation.
• Avoid perpendicular operation to the body.
• Communicate with the client during treatment and adjust the intensity and mode accordingly



Function: Slim Arm

1. Apply gel to the treatment area before operation.

2. Set the parameters:

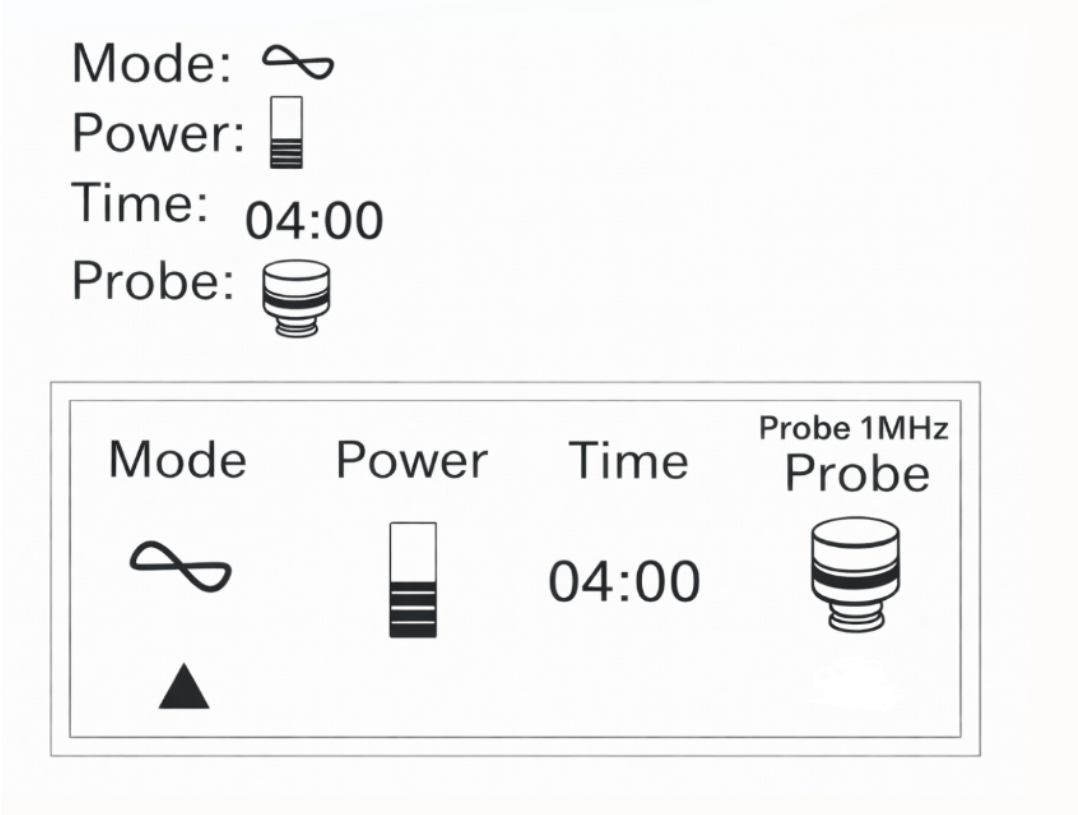

3. Operation method:


• Pinch the excess fat with one hand, hold the probe with the other hand, and move the probe from top to bottom or left to right over the fat.
• Avoid the arm bone during operation.
• Communicate with the client during treatment and adjust the intensity and mode accordingly.



Function: Slim Buttocks and Legs (Shape Modification)


1. Apply water-based gel to the treatment area before operation.

2. Set the parameters:

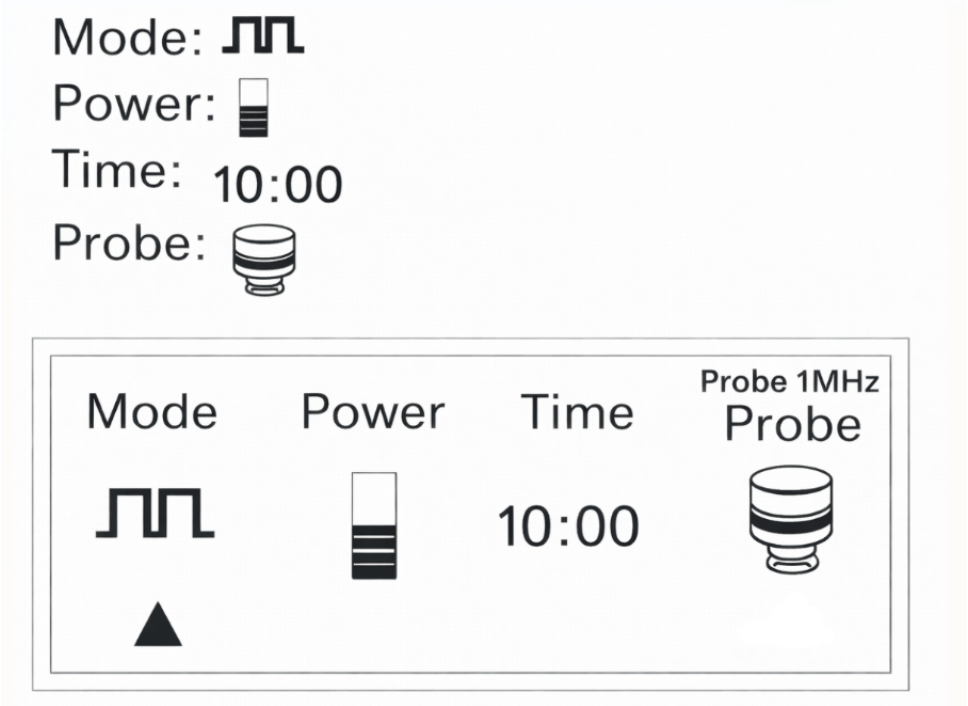

3. Operation method:

• Pinch the excess fat with one hand, hold the operation head with the other hand, and move the probe from top to bottom or left to right over the fat.
• Avoid the hip bone during operation.
• If the individual suffers from varicosity disease, do not perform the treatment. Consult a doctor.
• Communicate with the client during treatment and adjust the intensity and mode accordingly.

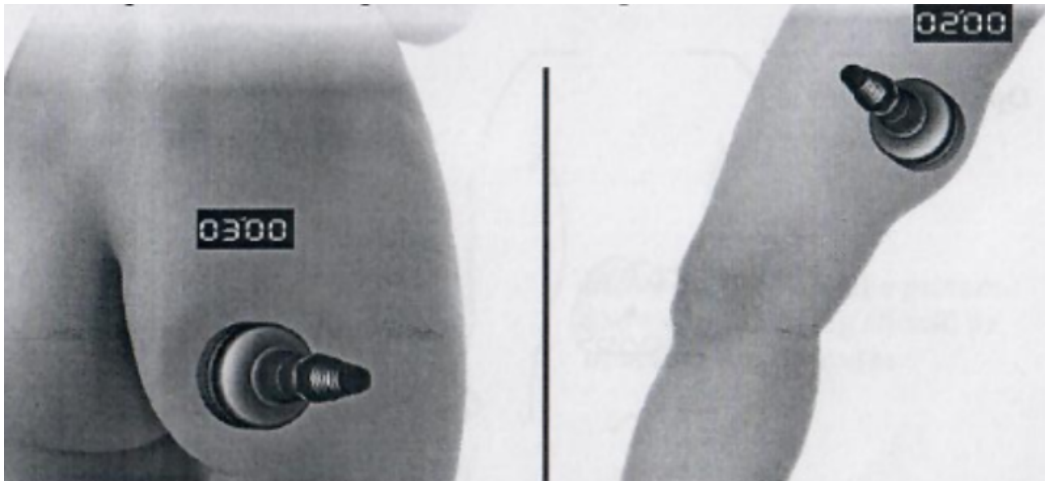


Ultrasonic Treatment

Function: Abdomen Massage


1. Massage the abdomen before operation and apply gel to the treatment area.

2. Set the parameters:

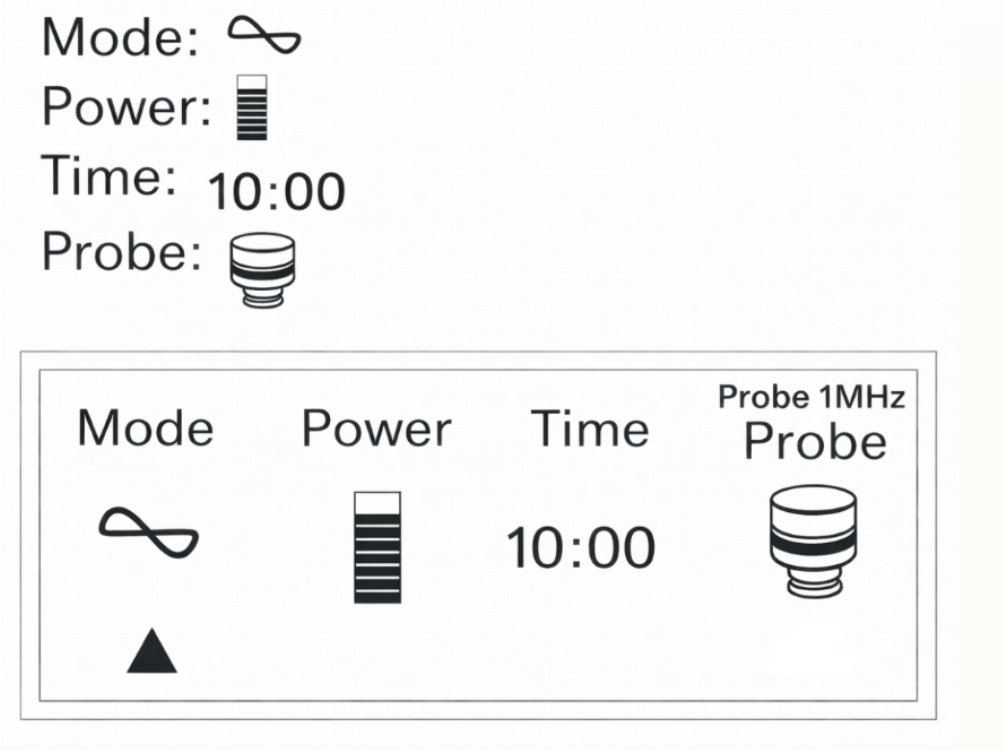

3. Operation method:


Move the probe in a circle, as shown in the image.

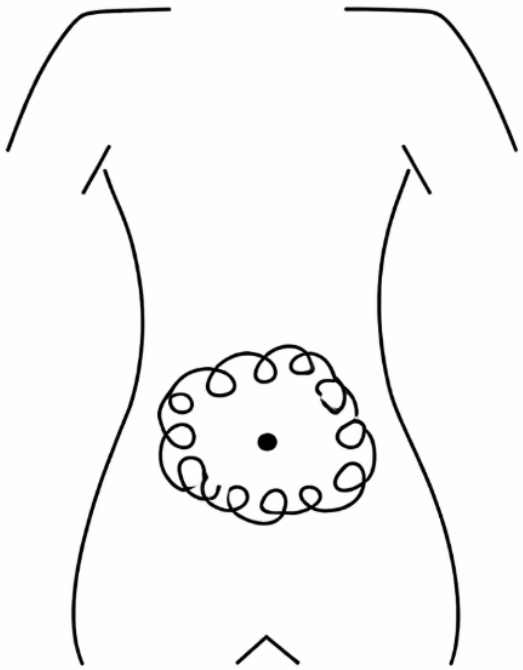

Function: Leg Shaping


1. Massage the legs before operation and apply gel to the treatment area.

2. Set the parameters:

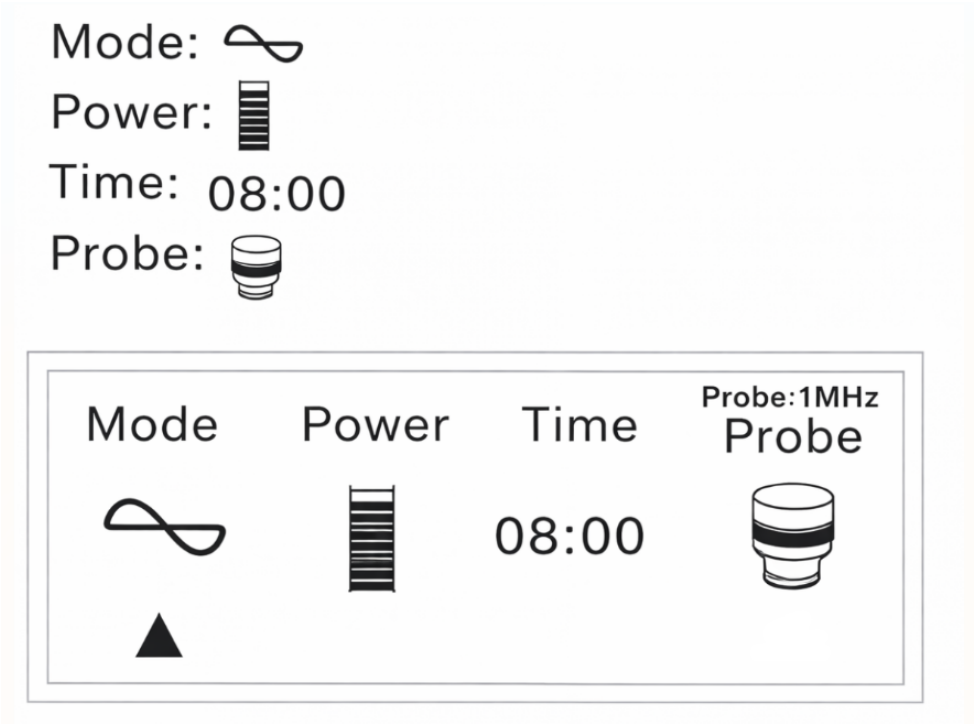

3. Operation method:


Move the probe as the picture shows and each leg should be operated for 2 minutes.

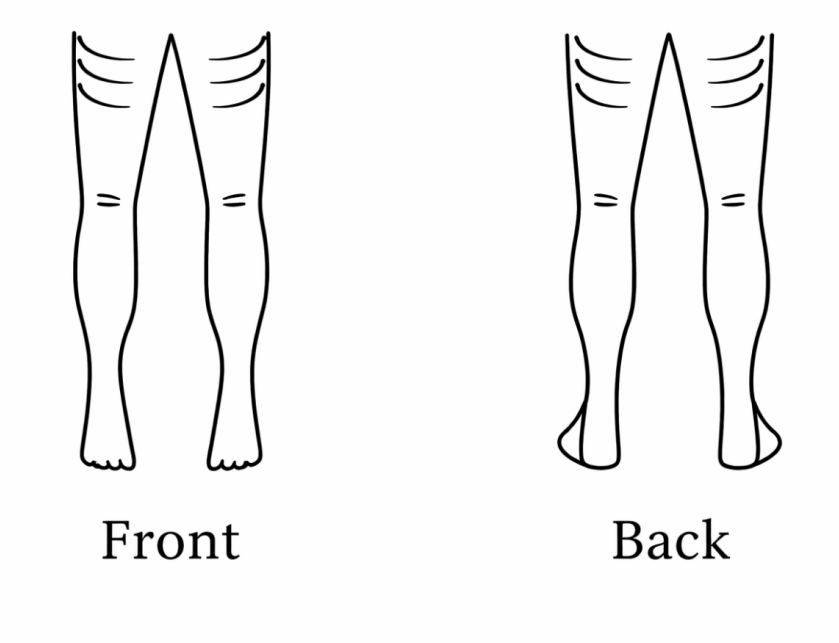

Breast Care


1. Massage on the breast before the operation and smear gel.

2. Set the parameters:

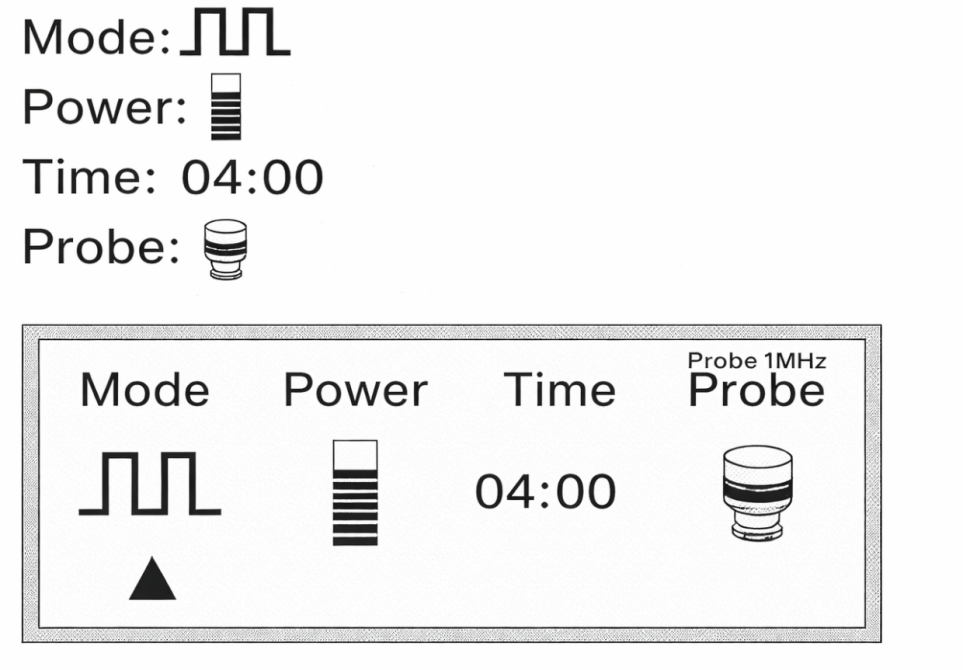

3. Operation method:

Lift breast outside in and from underneath to upper and each one should be operated for 2 minutes.

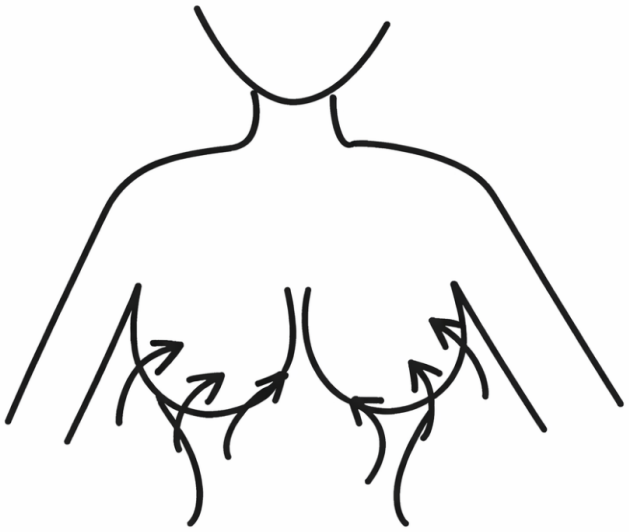

Troubleshooting

Problem	Cause	Solution
No power	Power not connected	Check power wire
Stops working	Overheating	Turn off and cool down
No response	Fuse damaged	Replace fuse

Technical Parameters

- Voltage: AC 110V
- Frequency: 60Hz
- Power: 120W
- Packing Size: 54 × 40 × 32 cm
- Gross Weight: 6.5 kg

Packing List

Item	Quantity
Main Machine	1
Big Probe	1
Small Probe	1
Power Cable	1
User Manual	1
Shelf	1
Stand Bar	4
Screws	2

Important Safety Notice

- Use indoors only.
- Keep away from water.
- Do not disassemble the device.
- Do not pull power cord forcefully.
- Turn off power when not in use.
- Keep out of reach of children.
- If the device malfunctions, contact service support.