LIPO X CAVITATION + RF VACUUM SKIN CARE MACHINE (RADIO FREQUENCY+ VACUUM)

(SKU18384)



SKIN+ACT

TOLL FREE: 1.800.418.0830 | WWW.SKINACT.COM WWW.SPAANDEQUIPMENT.COM | INTERNATIONAL: 818.834.6640

TABLE OF CONTENTS

SAFETY INSTRUCTIONS 03
TOOLS 05
GETTING STARTED 07
OPERATING INSTRUCTIONS 07
ADDITIONAL MAINTENANCE TIPS 10

THANK YOU FOR CHOOSING OUR PRODUCT!

Before using the device, we kindly ask you to carefully read the entire instruction manual provided. Please pay close attention to any warnings outlined in this manual. It's important to keep this instruction manual easily accessible at all times. If you pass the device to another individual, please ensure to provide them with the manual, as it is an integral part of the product. Please note that certain components of the product may differ from the images presented in catalogues, websites, brochures, etc. As part of our commitment to continually improve our products, the manufacturer reserves the right to modify features and/or components without prior notice.

THANK YOU AGAIN FOR YOUR PURCHASE. WE HOPE YOU ENJOY USING OUR PRODUCT!

SAFETY INSTRUCTIONS

IMPORTANT SAFEGUARDS

Before using your Lipo X machine, please read and understand all instructions in this manual. Improper use can lead to injury or damage.

GENERAL SAFETY

READ THE MANUAL:
Always refer to this manual for safe and effective use of your Lipo X machine.
INTENDED USE:
This machine is intended for personal use. It is not intended for people with reduced physical, sensory, or mental capabilities unless supervised by a qualified professional.
SUPERVISION:
Children should be supervised at all times to ensure they do not play with the machine.

WARNINGS

- Never disassemble, remodel, or attempt to repair the machine yourself. Contact a qualified service provider for any repairs.
- Do not place the machine near electronic or magnetic fields.
- Keep infants, children, and disabled individuals away from the machine, probe handles, accessories, and treatment area.
- Only use the rated voltage (230V, 50Hz). Using a higher voltage can cause fire, electric shock, or malfunction.
- Always insert the power plug completely and securely. Do not use a loose connection.
- Keep your hands dry when handling the power connector or machine. Wet hands can increase the risk of electric shock.
- If the probe handles or cord are damaged (including broken wires), do not use the machine. Contact a service provider for repairs.
- Do not use defective probe handles. This can cause skin damage.

SAFE OPERATION

- Do not use the machine in the following locations: shower rooms, kitchens, near humidifiers, or dusty environments.
- Do not use the machine if the power cord is damaged. A damaged cord should be replaced by a qualified professional to avoid hazards.
- Keep probe handles away from your eyes. This can cause eye pain.
- When not in use, unplug the power cord for safety.
- Do not use the machine with other devices at the same time. Additionally, do not use probes wrapped in cloth or paper.
- Use the probe handles only on bare skin. Do not use them around volatile materials (such as benzene or thinner).

- Keep the machine and power cord away from heaters. This can damage the cord and accessories, and may cause a fire or electric shock.
- Keep water or liquids away from the probe and machine.
- Avoid dropping or hitting the machine or probe handles. This can cause damage.
- If you experience any noise, malfunction, or pain during use, stop using the machine immediately, unplug the power cord, and contact a service provider.
- Do not use the machine during thunderstorms. Lightning strikes can cause power surges.

SAFE STORAGE

Store the machine in a cool, dry place away from direct sunlight and heat sources.
Store the machine on a flat surface to prevent falls.

PROHIBITED USE

DO NOT USE THE MACHINE IF YOU HAVE ANY OF THE FOLLOWING CONDITIONS:

- Acute illness, are intoxicated, are under the influence of sleeping pills, are overworked, are undergoing a medical examination, or are experiencing pain or symptoms.
- Do not use the machine if you have any implanted medical devices, such as pacemakers, implants, plastic surgery enhancements, or bone cement. This can cause malfunction of the medical device.
- Pregnant women, nursing mothers, epileptics, and people with tumors should not use the machine.
- People with the following conditions should not use the machine: acute inflammation, communicable diseases, unhealed surgical wounds, heart or kidney disease, diabetes, heart problems, brain or spinal issues, eye injuries, bleeding, infections, or who operate implanted medical devices.
- The machine should not be used by people who have recently undergone surgery, such as abdominal surgery, insertion of an IUD, or treatment for urinary incontinence.
- People with acute illnesses, fevers exceeding 38°C (100.4°F), blood pressure abnormalities, infectious diseases, tuberculosis, allergies, or hemophilia should not use the machine.
- People with atomic bomb disease, legal communicable diseases, facial melanosis, excessive internal heat, or those who frequently visit hospitals should not use the machine.
- People taking medication or children under 12 years old should not use the machine.

NOTE: PEOPLE WITH ANY MEDICAL CONDITIONS SHOULD CONSULT THEIR DOCTOR BEFORE USING THE LIPO X MACHINE.

- **KEEP CHILDREN AWAY FROM THE TREATMENT AREA.**
- **STOP USING THE MACHINE IF YOU EXPERIENCE ANY PAIN, SYMPTOMS, OR SKIN IRRITATION.**
- **IMPROPER USE OR REPETITIVE TREATMENT OF THE SAME AREA CAN CAUSE SKIN DAMAGE. IF YOU EXPERIENCE SKIN PROBLEMS, APPLY A COLD COMPRESS IMMEDIATELY AND CONSULT YOUR DOCTOR.**

Tools



Lipo X Machine (1 unit)



Vacuum & RF Handles (3 units): These are the handheld applicators used for the Vacuum & RF treatment mode.



Cavitation Handle (1 unit): This is the handheld applicator used for the Cavitation treatment mode.

▪ Upside of the body



Handle Holder

Touch Screeen

▪ Backside

Jog Dial



Handle Arm

Cavitation Handle Connector

Vacuum & RF Handle Connector

Suction Filter

Basket

GETTING STARTED

BEFORE YOU BEGIN

1. CHOOSE A SAFE ENVIRONMENT:

- Find a clean, flat surface to place the machine.
- Make sure children and pets cannot access the area during treatment.
- Avoid using the machine near other electrical appliances.
- Use the machine in a cool, dry environment.

2. PREPARE YOUR BODY:

- Remove all metal jewelry (watch, ring, necklace, bracelet, etc.) before treatment.
- Wear clothing without metal fasteners.

3. GET READY FOR TREATMENT:

- Plug the power cord securely into a wall outlet.
- Read the instructions carefully to ensure proper use.
- Important: Clean and disinfect the probe handles that will touch your skin before each use.

4. TREATMENT GEL (OPTIONAL):

- For a more comfortable treatment, apply a thin layer of ultrasound gel to the area you plan to treat.

Note: This machine is not intended for use on areas that have undergone surgery or have implants.

STARTING TREATMENT:

- Plug in the power cord.
- Turn on the power switch on the machine (refer to specific instructions for your model).

OPERATING INSTRUCTIONS

BEFORE YOU BEGIN YOUR TREATMENT, FOLLOW THESE STEPS:

1. Connect the Power Cord: Plug the power cord securely into a wall outlet.
2. Turn on the Machine: Locate the power switch on the back of the machine and turn it on (refer to specific instructions for your model).
3. Select Mode: The LCD screen will display "SELECT MODE."

PREPARING FOR TREATMENT

1. Handle Connection: Make sure the handle is properly connected to the designated port on the machine. Clean the handle with a dry or soft cloth before each use.
2. Treatment Cream:
3. Vacuum & RF Mode: Use only RF cream for this mode. Gels or other products can cause skin burns or malfunction.
4. Cavitation Mode: Use ultrasound gel for this mode.
5. Metal Jewelry: Remove all metal jewelry (watch, ring, necklace, bracelet, etc.) before treatment.

TREATMENT MODES

The Lipo X machine offers three treatment modes: Vacuum RF, Cavitation, and Vacuum & RF.

VACUUM RF MODE

1. Vacuum Level: Adjust the vacuum level on the screen (0 to 8).
2. RF Level: Adjust the RF level on the screen (1 to 10).
3. Vacuum Pattern: Choose your desired vacuum pattern (continuous or pulsed: 4Hz, 8Hz, 12Hz).
4. Treatment Time: Set the desired treatment time (up to 30 minutes).


CAVITATION MODE

1. Cavitation Level: Adjust the cavitation level on the screen (1 to 10).
2. Treatment Time: Set the desired treatment time (up to 30 minutes).


TREATMENT AREAS

This machine can be used to treat various areas of the body, including:


- Abdomen
- Back
- Thighs & Hips

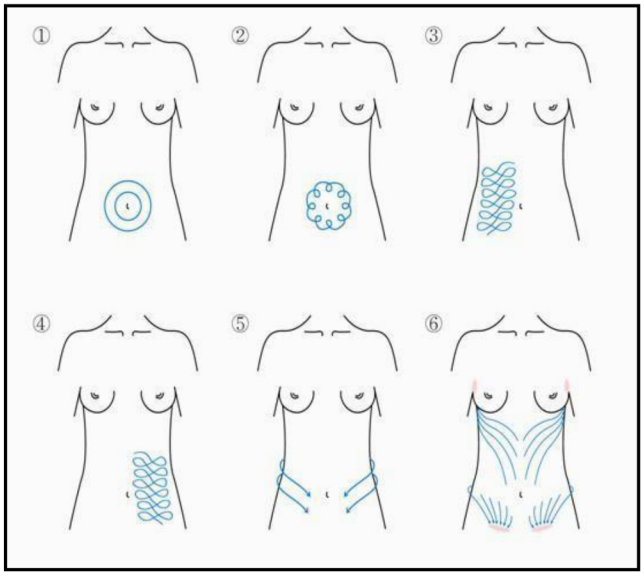

Abdomen

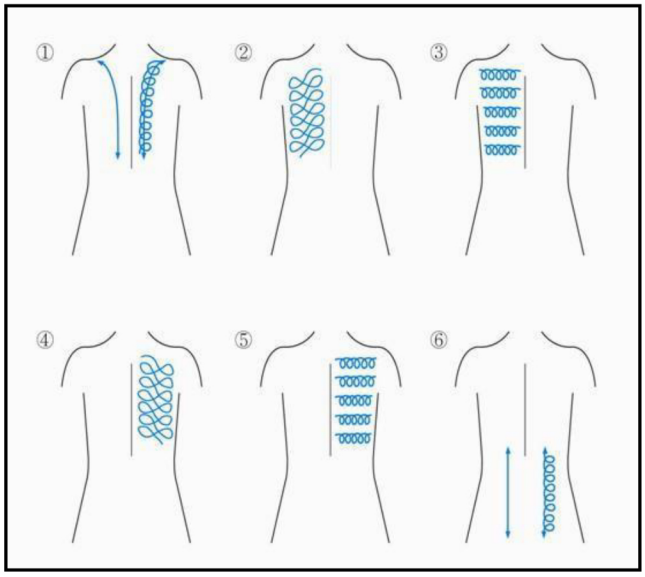

Back

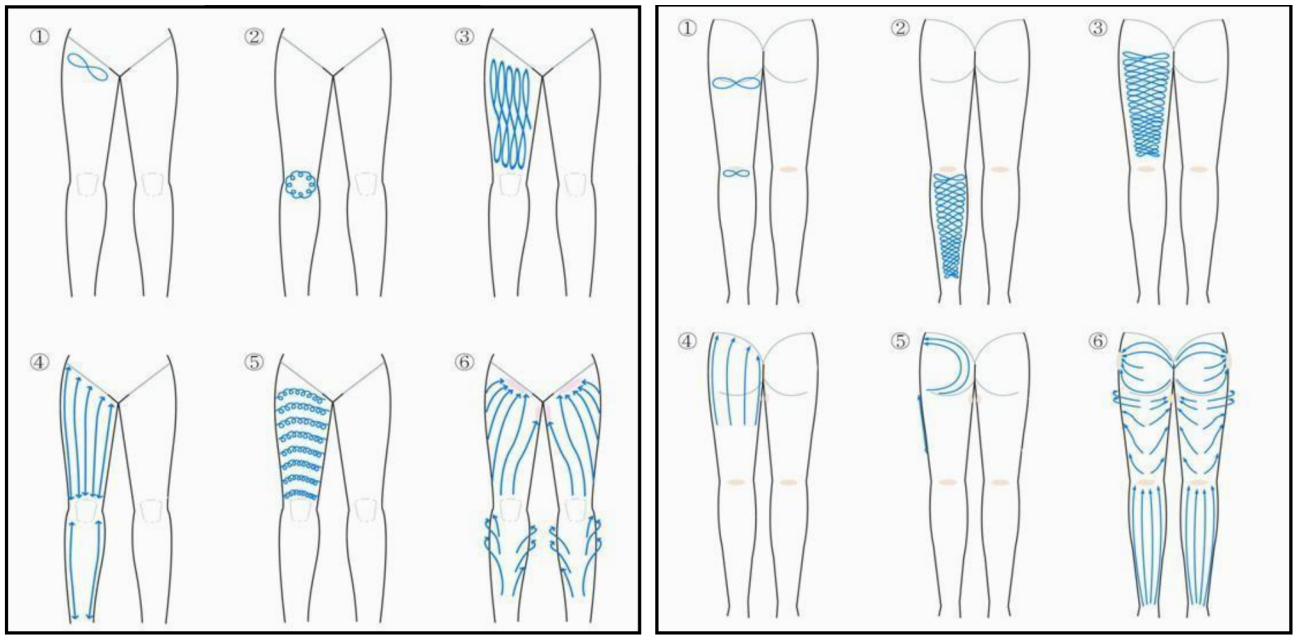

Thigh & Hip

STORAGE AND MAINTENANCE

- After use, clean the handle with a soft, dry cloth.
- Keep the handle surface clean and dry.
- Avoid storing the machine in direct sunlight, high temperatures, or high humidity environments.
- Do not repair or modify the machine yourself.
- Do not store the machine in a place with shocks, vibrations, or unstable conditions.

TURNING OFF THE MACHINE

1. After treatment, place the handle back on its cradle.
2. Turn off the power switch on the machine.
3. Unplug the power cord from the outlet and the machine.

CLEANING THE HANDLE

1. Wipe down the handle with a dry cloth after each use.
2. Turn off the machine after treatment.
3. Avoid storing the machine in direct sunlight, high temperatures, or high humidity environments.
4. Do not disassemble or modify the machine. If you experience any problems, stop using it and consult a technician.
5. Do not store the machine in an unstable or unsecured location.

ADDITIONAL MAINTENANCE TIPS

- Do not use flammable liquids (thinner, benzene) to clean the machine. This may cause discoloration or deformation.
- Keep the machine out of reach of children.
- Avoid using the machine near shocks or vibrations.
- Store the machine in a dry place out of direct sunlight when not in use (dust-free environment).
- Do not attempt to repair or modify the machine yourself.

REGULAR INSPECTION

- Before each use, inspect the machine and treatment components for any damage.
- If the machine hasn't been used for a while, test it to ensure proper operation before use.

IMPORTANT NOTE FOR VACUUM & RF MODE

When using the Vacuum & RF handle, start by using the RF function only for 4-5 minutes until the RF cream liquefies. Then, activate both the vacuum and RF functions together. Using unmelted RF cream can disrupt the vacuum function.

CLEANING THE HANDLE (WEEKLY OR EVERY 3 DAYS)

1. Prepare a cup of alcohol.
2. Turn off the vacuum function and set the level to 8.
3. Slowly pour a small amount of alcohol into the vacuum hole and cover the hole intermittently to allow absorption (repeat 3-4 times).
4. The alcohol will flow through the handpiece line and fill the bottle.
5. Turn the filter counterclockwise and detach it. Drain the contents, then turn the filter clockwise and reattach it.

SpaandEquipment offers a 1-year limited warranty on most equipment, covering malfunctions and manufacturer defects only (parts only, shipping not included). Warranty is void for improper use, wear & tear, alterations, or lack of professional installation for plumbing & electrical equipment (proof required). Customers are responsible for return shipping costs and damage during return shipment voids warranty (ship with insurance).

For details or questions, contact SpaandEquipment.com at 1.800.418.0830.

For further details regarding warranty coverage, please refer to our Warranty Information Policy on our website.
You can find it under the "Return/Shipping/Warranty" section.

SPECIFICATIONS AND TECHNICAL DATA

PRODUCT NAME:
Lipo X Cavitation + RF Vacuum Skin Care Machine
(Radio Frequency+ Vacuum) SKU18384

FUNCTION:
Combining the power of cavitation, radio frequency (RF), and vacuum technologies, this machine offers a revolutionary approach to skincare.

SPECIFICATIONS:
Radio frequency: 500 KHz, Cavitation: 27KHz
Power consumption: 40W, Vacuum Range: 650 mmhg