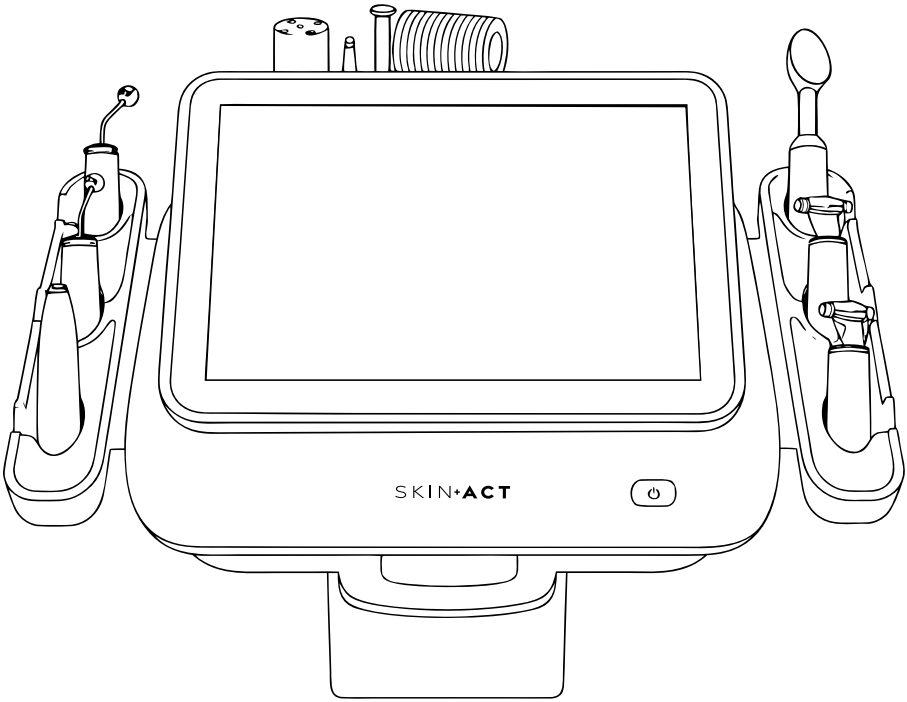
SKIN+ACT

Ultra 6 in 1 Microdermabrasion + Skin Scrubber + Bipolar RF + Mesotherapy + Cooling Treatment + Bio-Lift

PRODUCT MANUAL



SKU23181

SKINACT.COM

NOTICE

No part of this document may be photocopied, reproduced, or translated into any other language without prior written consent of Spa and Equipment/SkinAct.

The information in this document is subject to change without notice at any time and should not be construed as a commitment by Spa and Equipment/SkinAct

Spa and Equipment/SkinAct assumes no responsibility for any errors that may be in this document, nor does it make expressed or implied warranty with regard to this material, including, but not limited to, the implied warranties of merchant ability and fitness for a particular purpose.

Spa and Equipment/SkinAct shall not be liable for incidental or consequential damages arising out of the furnishing, performance, or use of this document and the program material which it describes.

Thank You For Purchasing This Product!

Please read the entire instruction manual carefully before using the product. Take note of any warnings included in this manual.

Always keep this instruction manual handy and if you give the device to another person, hand over the manual as it is an essential part of the product.

Some components of the product may differ from the image that appears in catalogues, websites, brochures, ect..

In order to enhance the product, the manufacturer reserves the right to modify its features and/or components without prior notice.

Copyright © 2026 SkinAct, All Rights Reserved

TABLE OF CONTENTS

Disclaimer 4

Contraindications & Precautions 5

Areas to Avoid & Important Safety Notes 6

Included Items 7

Benefits of Each Handle 8

Operating Instructions 9

Treatment Guidelines

1. Mircodermabrasion 11
2. Skin Scrubber 12
3. Bipolar RF 13
4. Needleless Mesotherapy Facial 14
5. Needleless Mesotherapy Eye 15
6. Cooling Treatment 16
7. BIO Round Microcurrent Eye 17
8. BIO Roller Microcurrent Face 18

Important Notes 20

Troubleshooting 21

Specifications 22

Warranty Information 23

DISCLAIMER

- This product has been designed to be used by esthetic professionals at spas and salons, it should not be used for other purposes.
- Please note that any misuse of the device entails the loss of the guarantee.
- Do not make any modification to the device without the authorization.
- We shall not be held liable for any material or personal damage due to the misuse of the product.
- Documents are made available without warranty of any kind. They may be updated, altered, expanded, or removed at any time. Skin Act does not warrant or guarantee any of the processes described herein or perform any independent analysis in connection with guidelines provided.
- Readers are expressly warned to consider and adopt all safety precautions indicated herein and to avoid all potential hazards. By following the instructions provided, the reader willingly assumes all risks in connection with such instructions.
- If the reader has questions about any of the guidelines provided by SkinAct we recommend they contact their nearest Esthetician Training Center to obtain more explicit instruction on Facial Machine Usage.

Contraindications

THIS DEVICE SHOULD NOT BE USED ON CLIENTS WITH:

- Pacemakers, metallic implants, or other electronic medical devices.
- Heart conditions or a history of heart disease.
- Pregnancy.
- Inflamed, irritated, or damaged skin.
- Eczema, dermatitis, swelling, or sunburn.
- Clients who have received hydroxy acid treatments, laser resurfacing, chemical peels, or wound-healing procedures within the past 3 months.
- Over areas with permanent or temporary dermal fillers unless approved by a physician.
- Clients with skin cancer, suspicious lesions, or precancerous conditions.
- Clients currently using blood-thinning medications or who have taken isotretinoin (retinoic acid) within the past 2 months.
- Clients with asthma, cold, flu or upset stomach.
- Clients with epilepsy, alcoholism, ulcers or digestive system disorders

Precautions

- **Inspect the Device:** Check for any visible damage to the device or its power cable before and after each use.
- **Unplug When Not in Use:** Always disconnect the device from the power source before cleaning, storing, or performing maintenance.
- **Avoid Humidity:** Do not operate the device in excessively humid environments.

- **Position Cables Safely:** Ensure the power cable is positioned to prevent tripping hazards and is plugged into a grounded socket.
- **Keep Away from Children:** The device and its accessories should be stored securely out of reach.
- **Report Issues Promptly:** If you notice abnormal functioning, contact your distributor or an authorized technician immediately.
- **Remove Jewelry:** All jewelry and metal piercings must be removed prior to performing microcurrent treatments.








Areas To Avoid Treatment

- Sensitive Skin
- Skin rashes, damaged, inflamed, or infected areas
- Surgical Scars less than 12 months old
- Swollen Skin
- Eyeballs (probes should never point directly at them)
- Genitals







Important

- Always start with the lowest settings and gradually increase based on your skin's reaction.
- Mild swelling and redness may occur after treatment but should disappear within a few hours.
- Overly aggressive techniques can cause temporary flaking or bleeding.
- Avoid microdermabrasion function on eyelids (keep them closed and covered during treatment).
- Certain areas are not suitable for treatment: skin tumors, moles, birthmarks, lips, eyes, herpes, skin cancer and liver spots.

Included Items

Qty	Part Name	Image
1	Host Machine	
1	Skin Scrubber	
1	Cooling Therapy Hammer	
1	Mesotherapy Eye Tool	
2	BIO Round	
1	BIO Roller	
1	Microdermabrasion Pen	
1	Bipolar RF	
1	Mesotherapy Face Tool	

Benefits of Each Handle

Microdermabrasion Gently exfoliates the skin to remove dead cells and improve skin texture.	
Skin Scrubber Deeply cleans pores to remove dirt and oil. Helps to reduce acne, remove blackheads, dimmish wrinkles and more.	
Bipolar RF (Radio Frequency) Improves skin elasticity and reduces wrinkles. Delivers controlled radio frequency energy to the skin and promoting collagen promotion.	
Needleless Mesotherapy Increases collagen and promotes better product absorptions. Two different tools for larger areas and for around the eyes.	
Cooling Treatment Soothes and calms the skin, reducing redness, inflammation, and irritation after other treatments or exposure to environmental.	
Microcurrent BIO lift Reduces wrinkles and improves skin elasticity and pushes products deeper into the skin. Two different tools for larger areas and for around the eyes.	

Operating Instructions

1. Locate the ports on the back of the main unit and connect each handle to its corresponding port, matching the handle to the icon displayed next to it.
2. Plug in host machine, flip the black switch behind the home screen and press the power button on the front.
3. The home screen will display the following available handles:

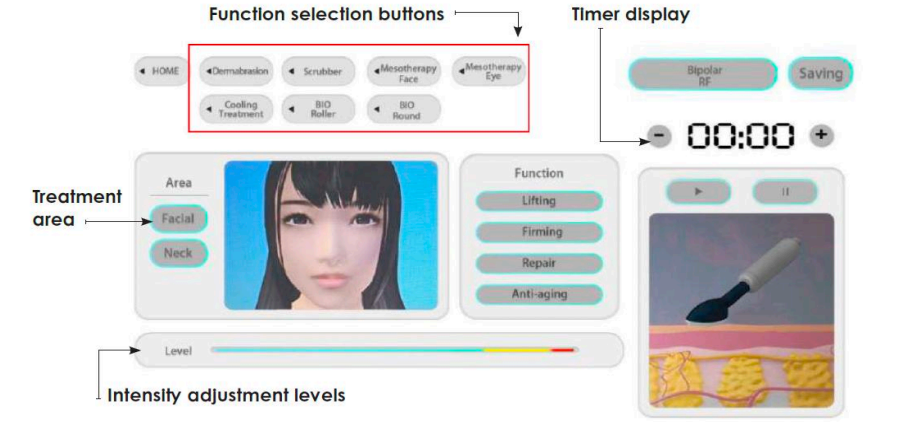
- Dermabrasion, Scrubber, Bipolar RF, Mesotherapy Face, Mesotherapy Eye, Cooling treatment, BIO Roller and BIO Round



3. Press a handle function on the screen and select your desired handle attachment. The treatment screen will appear, showing the following controls:

- Treatment Area: Face or Neck
- Function Mode: Lifting, Firming, Repair, or Anti-Aging
- Intensity Level: Adjust according to client comfort and skin condition
- Treatment Time: Set the desired session duration using the timer controls

4. Configure your session settings and press start to start the treatment.




5. Tap Saving to store your current settings. When prompted with “Sure to save?” , select Yes to confirm.



Treatment Guidelines

1. Mircodermabrasion

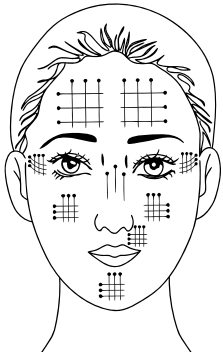Follow the movement directions shown in the examples.



Preparing for Treatment

1. **Choose the Dermabrasion Attachment:** Select the appropriate attachment for the desired treatment area.
2. **Set Treatment Time:** Set the treatment time for 15 - 20 minutes.
3. **Adjust Vacuum Level:** The vacuum level should be adjusted based on your client's comfort level. Start with a lower suction for sensitive areas like the eye area.
4. Ensure the filters are clean and in place for proper suction

Treatment

- **Test Suction**

Before applying the face, test the suction level on your arm to ensure its comfortable.

- **Treatment Technique**

Move the tip in smooth, circular motions, avoiding any area for more than 15 seconds. This helps prevent irritation or bruising.

- **Post-Treatment Care**

Clean the diamond tip with a brush and water after use. Disinfect it by soaking it in a 75% alcohol solution for 15 minutes, followed by wiping it dry and placing it in a UV sterilizer.

Important Note: These are general guidelines. Communicate with your client throughout the treatment and adjust settings based on their comfort and specific needs.

2. Skin Scrubber

Follow the movement directions shown in the examples.



Treatment

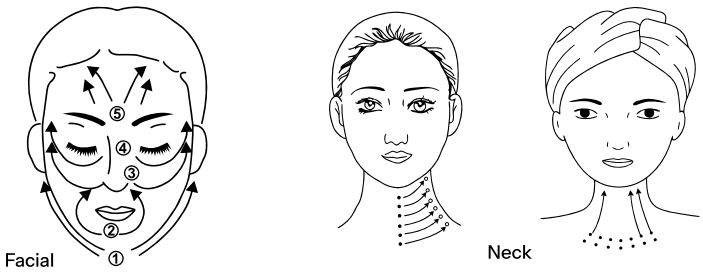
1. **Choose Scrubber Attachment:** Select the appropriate attachment for your desired treatment.
2. **Adjust Settings:** Set the treatment time for 15 - 20 minutes.
3. Choose the treatment area, function, mode, and intensity level based on your client's needs and preferences.

- Operating at 28,000 Hz, the device deeply cleanses, massages, and stimulates skin cells to reduce spots and wrinkles.

Important Note: These are general guidelines. Communicate with your client throughout the treatment and adjust settings based on their comfort and specific needs.

3. Bipolar RF

Follow the movement directions shown in the examples.



Facial

1. **Choose Bipolar RF:** Select the appropriate attachment for facial treatment.
2. **Set Treatment Time:** Set the treatment time for 15 - 20 minutes.
3. **Adjust Intensity:** Adjust the intensity level based on your client's comfort and skin sensitivity.
4. **Apply Medium:** Apply a conductive medium to the treatment area.
5. **Move Probe:** Glide the probe in the correct areas in smooth, circular motions.

Neck

1. **Set Treatment Time:** Set the treatment for 15 - 20 minutes,
2. **Adjust Intensity:** Adjust the intensity level based on your client's comfort and skin sensitivity.
3. **Apply Medium:** Apply a conductive medium to the neck area.
4. **Move Probe:** Glide the probe in the correct areas in smooth, upward motions.

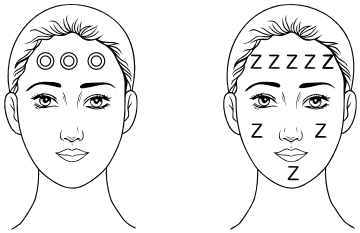
IMPORTANT

Avoid Prolonged Contact: Do not keep the probe stationary in one place for an extended period.

Monitor Client Comfort: Continuously communicate with your client during the treatment and adjust.

4. Needleless Mesotherapy Facial

Follow the movement directions shown in the examples.



1. **Choose Mesotherapy:** Select the appropriate attachment for your desired treatment.
2. **Set Treatment Time:** Set the treatment time for 15 - 20 minutes.
3. **Adjust Intensity:** Adjust the intensity level based on your client's comfort and skin sensitivity.
4. **Apply Product:** Apply a suitable skincare product directly to the treatment area, or fill the handle's bottle with skincare product by twisting the handle to remove the bottle, filling it, and reattaching securely before use.
5. **Move Probe:** Glide the probe over facial skin in smooth, circular motions in the directions shown in the figure.

IMPORTANT

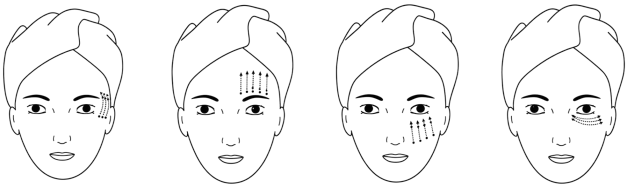
Monitor Client Comfort: Continuously communicate with your client during the treatment and adjust.

Avoid Prolonged Contact: Do nor keep probe stationary in one place for an extended period.

Consult with a Dermatologist: If you have any concerns about using mesotherapy on your clients, it is recommended to consult with a dermatologist.

5. Needleless Mesotherapy Eye

Follow the movement directions shown in the examples.



1. **Choose Mesotherapy:** Select the appropriate attachment for your desired treatment.
2. **Set Treatment Time:** Set the treatment time for 10 - 15 minutes.
3. **Adjust Intensity:** Adjust the intensity level based on your client's comfort and skin sensitivity.
4. **Apply Product:** Apply a skincare product to the treatment area.
5. **Move Probe:** Glide the probe over facial skin in smooth, circular motions in the direction as shown in the figure above.

IMPORTANT

Monitor Client Comfort: Continuously communicate with your client during the treatment and adjust.

Avoid Prolonged Contact: Do nor keep probe stationary in one place for an extended period.

Consult with a Dermatologist: If you have any concerns about using mesotherapy on your clients, it is recommended to consult with a dermatologist.

6. Cooling Treatment

Follow the movement directions shown in the examples.




1. **Choose Cooling Hammer:** Select the appropriate attachment for facial cooling treatment.
2. **Set Treatment Time:** Set the treatment time for 10 - 15 minutes.
3. **Adjust Intensity:** Adjust the intensity level based on your client's comfort and skin sensitivity.
4. **Move Probe:** Glide the probe in the correct areas shown in the figure above with smooth, circular motions.

IMPORTANT

Monitor Client Comfort: Continuously communicate with your client during the treatment and adjust settings as needed.
Avoid Prolonged Contact: Do not keep the probe stationary in one place for extended period

7. BIO Round Microcurrent Eye

Follow the movement directions shown in the examples.




1. **Choose BIO Round:** Select the appropriate attachment for BIO Round treatment.
2. **Set Treatment Time:** Set the treatment time for 10 - 15 minutes.
3. **Adjust Intensity:** Adjust the intensity level based on your client's comfort and skin sensitivity.
4. **Position Probe:** Begin at the inner corner of the eye, along the orbital bone.
5. **Glide Outward:** Move the probe smoothly outward and upward along the orbital bone towards the temple engaging the levator muscles to life and toner the eye area.
6. **Apply Light Pressure:** Use gentle, consistent pressure throughout the movement. For the eyebrow area, an optional pinch technique can be applied to target the depressor muscles.

IMPORTANT

Monitor Client Comfort: Continuously communicate with your client during the treatment and adjust settings as needed.
Avoid Eye Contact: Keep the probe on the orbital bone at all times and avoid direct contact with eyeball.

7. BIO Roller Microcurrent Face

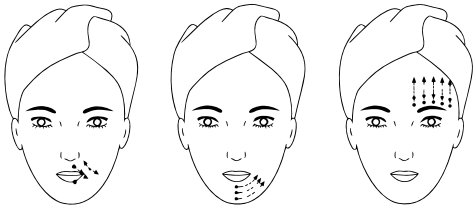Follow the movement directions shown in the examples.



1. **Choose BIO Roller:** Select the appropriate attachment for BIO Roller treatment.
2. **Set Treatment Time:** Set the treatment time for 10 - 15 minutes.
3. **Adjust Intensity:** Adjust the intensity level based on your client's comfort and skin sensitivity.
4. **Apply Product:** Apply a skincare product to the treatment area.

Nasolabial Folds:

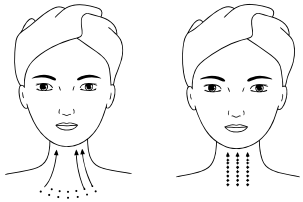
- **Lift and sculpt:** Glide the probe diagonally upward from the sides of the nostrils towards the cheekbones, engaging the levator labii superioris to smooth and lift the nasolabial fold area.

Jawline:

- **Position Probe:** Begin at the center of the chin along the jawline
- **Glide Upward:** Move the probe smoothly upward along the jawline toward the back of the ear stimulating the depressor anguli oris to improve definition and contour.
- **Pinch Technique:** Apply the optional pinch technique along the jawline to further engage the underlying muscles and enhance definition

Forehead:

- **Glide Upward:** Beginning at the center of the eyebrows, move the probe smooth upward towards the hairline, engaging the frontalis muscle to lift and smooth the forehead and reduce the appearance of horizontal lines.



Neck:

- **Stroke Upward:** Using low to moderate intensity, move the probe in smooth, upward strokes from the base of the neck toward the jawline, targeting the platysma muscle to life and firm the skin.
- **Apply Gentle Pressure:** Maintain light, consistent pressure throughout due to sensitivity of the neck area.

IMPORTANT: Avoid using the device over the Thyroid area, as stimulation in this region may pose serious health risks.

Important Notes

- **Cleanse the skin:** Before treatment, ensure the skin is clean and free of makeup or other products.
- **Appy a serum:** For enhanced results, apply a serum or a water-based conductive gel before using the both microcurrent handles. All SkinAct serums are recommended for usage.
- **Monitor Client Comfort:** Continuously check with your client to ensure they are comfortable throughout the treatment.
- **Avoid sensitive areas:** Avoid rolling the device over areas with broken skin, moles, warts or other skin conditions.
- **Clean and disinfect:** After the treatment, clean and disinfect the device and attachments.

Troubleshooting

Machine does not respond when powered on
Solution: Ensure the power supple is securely connected to the machine. Confirm the power switch is turn on.

No Output
Solution: Check that the attachment is properly and fully connected to the correct output port

Machine overheats during use
Solution: Power off the unit immediately and allow it to cool down naturally before resuming use. If overheating persists, have a qualified technician check that the voltage supply meets the required specifications

No Power
Inspect the fuse and replace it if damaged.

Specifications

Product Name:	Ultra 6 in 1 Microdermabrasion + Skin Scrubber + Bipolar RF + Mesotherapy + Cooling Treatment + Bio-Lift
Voltage:	AC150V/250V
Frequency:	50Hz
Power Consumption:	75W
Dimensions(L*W*H):	14.2x12x6.5 in
Net Weight:	27lbs

Warranty Information

The manufacturer (the “warrantor”) warrants to the original purchaser that this equipment will be free from defects under normal and proper operation for a period of one (1) year from the date of purchase. This warranty covers all parts and labor for that one (1) year period. This warranty shall not apply to any equipment that has been subjected to abuse, misuse and alteration of any type or to any defect or damage caused by repair, replacement, substitution, or use with parts other than parts approved by the manufacturer. The manufacturer shall not be liable for the loss of use of this equipment, loss of time or business, inconvenience or any other indirect, consequential, special or incidental damages due to defects covered by this warranty or any implied warranty. To implement this warranty, contact the dealer from whom you purchased the equipment. If necessary, you will be asked to return all, or the appropriate part, of the equipment. If warranted, the repairs will be performed at no charge and the equipment returned to you. Unit owner must prepay all shipping costs when returning items for warranty service. This limited warranty is the only written or express warranty given by the manufacturer. This warranty gives you specific legal rights but you may also have other rights, which may vary from state to state or province to province.

SKIN+ACT

Phone: 1-800-418-0830
Email: info@skinact.com
Website: skinact.com