
SKIN+ACT

High Frequency Table Top Facial Unit HF

PRODUCT MANUAL

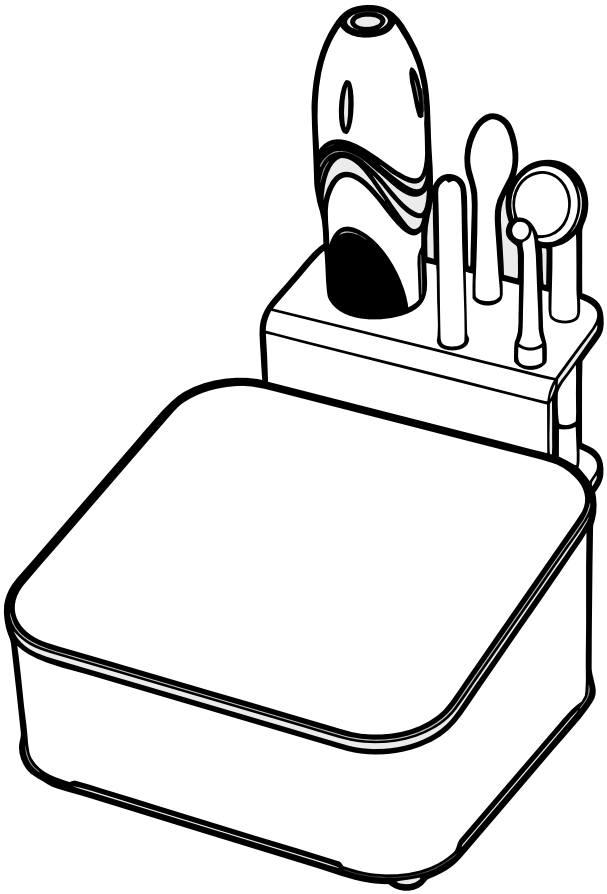

SKU25347

SKINACT.COM

NOTICE

No part of this document may be photocopied, reproduced, or translated into any other language with out prior written consent of Spa and Equipment/SkinAct.

The information in this document is subject to change without notice at any time and should not be construed as a commitment by Spa and Equipment/SkinAct

Spa and Equipment/SkinAct assumes no responsibility for any errors that may be in this document, nor does it make expressed or implied warranty with regard to this material, including, but not limited to, the implied warranties of merchantability and fitness for a particular purpose.

Spa and Equipment/SkinAct shall not be liable for incidental or consequential damages arising out of the furnishing, performance, or use of this document and the program material which it describes.

Thank You For Purchasing This Product!

Please read the entire instruction manual carefully before using the product. Take note of any warnings included in this manual.

Always keep this instruction manual handy and if you give the device to another person, hand over the manual as it is an essential part of the product.

Some components of the product may differ from the image that appears in catalogues, websites, brochures, etc.

In order to enhance the product, the manufacturer reserves the right to modify its features and/or components without prior notice.

Copyright © 2026 SkinAct, All Rights Reserved

TABLE OF CONTENTS

Disclaimer 4

Contraindications & Precautions 5

Electrotherapy Operation Guidelines 6

Safety During Operation 6

Safety Tips 7

Warnings 8

Included Items 9

Device Components 10

Glass Electrotherapy Tubes 11

Touch Panel 12

Device Assembly 13

Direct Electrotherapy 14

Effects of Direct Electrotherapy & Indirect Electrotherapy 15

Effects of Indirect Electrotherapy & Specifications 16

Warranty 17

DISCLAIMER

- This product has been designed to be used by esthetic professionals at spas and salons, it should not be used for other purposes.
- Please note that any misuse of the device entails the loss of the guarantee.
- Do not make any modification to the device without the authorization.
- We shall not be held liable for any material or personal damage due to the misuse of the product.
- Documents are made available without warranty of any kind. They may be updated, altered, expanded, or removed at any time. Skin Act does not warrant or guarantee any of the processes described herein or perform any independent analysis in connection with guidelines provided.
- Readers are expressly warned to consider and adopt all safety precautions indicated herein and to avoid all potential hazards. By following the instructions provided, the reader willingly assumes all risks in connection with such instructions.
- If the reader has questions about any of the guidelines provided by SkinAct we recommend they contact their nearest Esthetician Training Center to obtain more explicit instruction on Facial Machine Usage.

Contraindications

THIS DEVICE SHOULD NOT BE USED ON CLIENTS WITH:

- Pacemakers, metallic implants, or other electronic medical devices.
- Heart conditions or a history of heart disease.
- Pregnancy.
- Inflamed, irritated, or damaged skin.
- Severe acne rosacea or vascular conditions.
- Epilepsy or other seizure disorders.
- Clients undergoing medical treatments or with underlying health conditions must obtain prior clearance from a physician.

Precautions

- **Inspect the Device:** Check for any visible damage to the device or its power cable before and after each use.
- **Unplug When Not in Use:** Always disconnect the device from the power source before cleaning, storing, or performing maintenance.
- **Avoid Humidity:** Do not operate the device in bathrooms or other excessively humid environments.
- **Position Cables Safely:** Ensure the power cable is positioned to prevent tripping hazards and is plugged into a grounded socket.
- **Keep Away from Children:** The device and its accessories should be stored securely out of reach.
- **Report Issues Promptly:** If you notice abnormal functioning, contact your distributor or an authorized technician immediately.

Electrotherapy Operation Guidelines

- **Normal Operation:** The electrotherapy handle emits a continuous “beep” sound during use.
- **Sparking (Direct Use):** Small sparks may occur if the electrode is slightly away from the skin, which may cause mild discomfort.
- **Energy Adjustment:** Begin at the lowest energy level before bringing the electrode into contact with the skin, then increase gradually.
- **Sensitive Skin:** If discomfort occurs, place a dry cotton gauze over the treatment area to reduce irritation.
- **Skin Contact:** Ensure the electrode maintains full contact with the skin to prevent excessive sparking.
- **Treatment Duration:**
- **Oily skin:** approximately 8 minutes
- **Dry skin:** 3–5 minutes
- **Intensity Level:** Use higher intensity for oily skin and lower intensity for dry skin.
- **Indirect Use:** Maintain contact with the client’s skin during indirect electrotherapy to ensure consistent current flow.

Safety During Operation

- **Start Procedure:** Press Start only after the electrode is in contact with the skin, then gradually increase energy.
- **Removal Procedure:** Before removing the electrode, reduce energy to the minimum and press **Off** to stop output.
- **Power Control:** Ensure the device is turned off before installing or removing glass electrodes.
- **Electrode Hygiene:** Keep all glass electrodes clean and dry and disinfected before and after each use.

- **Handle Cleaning:** Clean the electrotherapy handle with a dry cloth only. Do not wash it with water.
- **Oil Removal:** If oil residue is present, wipe with anhydrous alcohol and store in a dry place.



Safety Tips

- **Power Supply:** Ensure the device is connected to a properly installed outlet with the correct voltage.
- **Accessibility:** Use outlets that allow quick disconnection in case of emergency.
- **Unplugging:** Always unplug by holding the plug, not the power cord.
- **Repairs:** Do not attempt to open or repair the device. Only qualified technicians should perform repairs.
- **Damage Check:** Do not use the device if the power cord or unit is visibly damaged.
- **Wet Hands:** Do not touch the device or power cord with wet hands.
- **Skin Check:** Do not use the device on irritated, inflamed, or infected skin areas
- **Power Stability:** Avoid using the device during power fluctuations or unstable electrical supply.


Warnings

- **Metal Objects:** Do not allow customers to touch metal objects during high-frequency electrotherapy. Remove all metal accessories before treatment.
- **Restricted Use:** Do not use this device on individuals with sensitive skin, skin discoloration, rosacea, wounds, pregnant individuals, or those with medical devices such as pacemakers.
- **Product Use:** Don't use skincare products containing alcohol during treatment. If needed, apply alcohol-based products only after electrotherapy.
- **Eye Safety:** Never point any electrotherapy electrode directly at the eyes.
- **Device Operation:** Do not touch the electrotherapy unit or output interface while the device is powered on.
- **Professional Use:** This device should be operated by trained professionals only.
- **Interference:** Keep the device away from other electronic equipment to avoid interference during operation.
- **Malfunction**: If any abnormalities occur, stop use immediately and contact a qualified technician. Do not attempt to open or repair the device yourself.
- **Environment:** Do not use the device in bathrooms or damp environments
- **Storage Safety:** Keep the device away from flammable or explosive materials.

Included Items


Qty	Part Name	Image
1	High Frequency Unit	
1	Attachment Rack	
1	High-Frequency Electrotherapy Handle	
1	Mushroom-Shape Glass Electrotherapy Tube	
1	Spoon-Shape Glass Electrotherapy Tube	
1	Spot Glass Electrotherapy Tube	
1	Straight-Bar Glass Electrotherapy Tube	
1	Power Cable	

Device Components

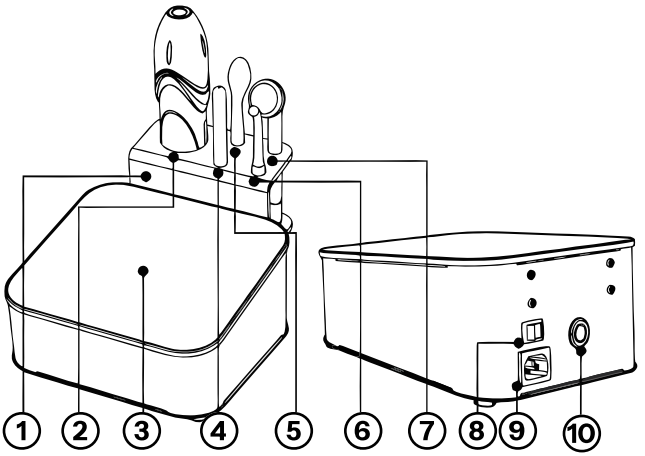


1. Attachment Rack
2. High-Frequency Handle
3. Control Panel
4. Rod (Straight) Electrode
5. Spoon Electrode
6. Spot Electrode
7. Mushroom Electrode
8. Power Switch
9. Electric Socket
10. Output Socket

High-Frequency Electrotherapy Handle

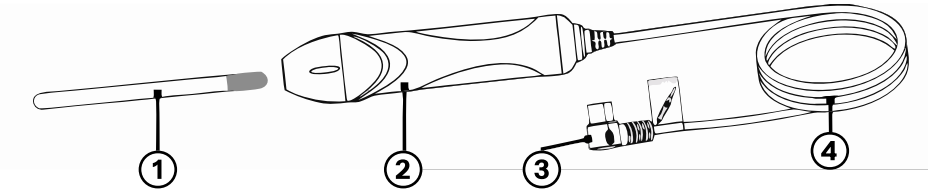


1. Electrotherapy Tube
2. Handle
3. Plug for Electrotherapy Handle
4. Electrotherapy handle flexible cable

Glass Electrotherapy Tubes

	Mushroom Electrode: Used for larger areas (Face & Neck)
	Spoon Electrode: Used for medium areas (Nose & Jawline)
	Spot Electrode: Used for small localized areas(Blemishes)
	Rod Electrode: Used for general & contour application areas

Assembly and Disassembly of the Electrotherapy Tube

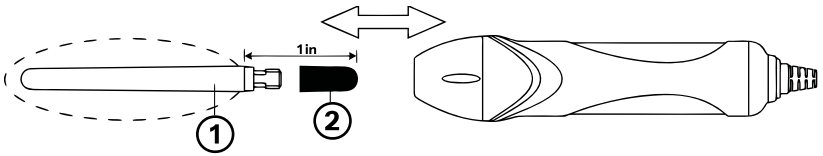


1. Glass Electrode
2. Metal Electrode

Instructions:


- When assembling or disassembling the electrotherapy tube, hold only the areas indicated by the dotted line.
- Keep your hand at least 30 mm away from the metal electrode at all times


Touch Panel

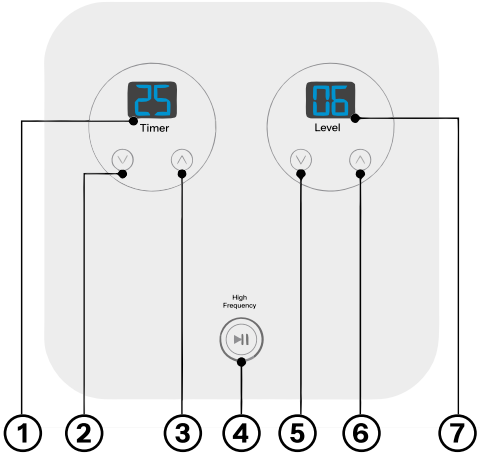


1. Timer Display
2. Decrease Timer
3. Increase Timer
4. Start/Pause
5. Decrease Energy Level
6. Increase Energy Level
7. Power Level Display

Device Assembly





1. Secure the attachment rack to the back of the main unit using screws, following the direction of the arrows.
2. Place each attachment onto the rack.
3. Plug the handles into the corresponding output ports on the front of the main unit. Preparation is now complete.
4. Connect the power cord to the main unit.

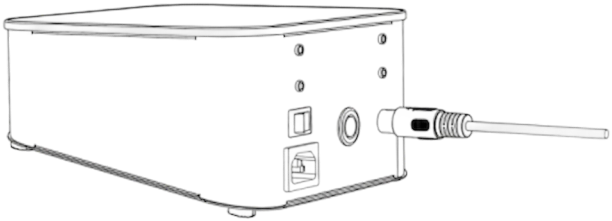


5. Flip the power switch on to enter standby mode. The time display will show “15,” and the energy display will show “1.”
6. In standby mode, press the Start/Pause button to begin operation. Settings can be adjusted while in standby mode.
7. Use the Timer Increase/Decrease buttons to adjust the operating time. The adjustable range is 1 to 30 minutes.
8. Use the Level Increase/Decrease buttons to adjust the energy output. The adjustable range is Level 1 to Level 9.

9. You can start or pause operation at any time by pressing the Start/Pause button while in standby or during operation

How to Use - Direct Electrotherapy

1. Hold the high-frequency electrotherapy handle by the designated grip area (as shown in the figure). Do not touch the glass tube with your hands, or keep contact to a minimum. Turn on the main power and set the energy **Level** to the lowest setting.

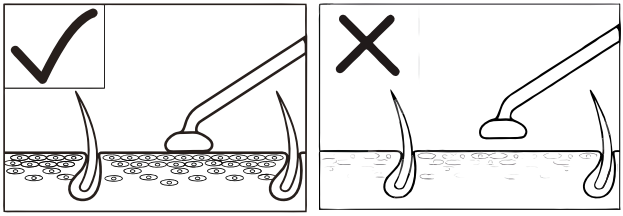

2. Place the glass electrotherapy tube in proper contact with the treatment area, then press the Start button to begin operation.
3. Gradually increase the energy by pressing **Level** The glass tube will generate ionized light and output high-frequency current.
   If a skincare product (such as cream or mask) has been applied, gently move the tube across the skin—starting from the neck and moving upward to the forehead, face, cheeks, and nose.
   Adjust the energy Level as needed during use. The generated heat provides a soothing effect, while also offering antibacterial benefits, making it suitable for oily and acne-prone skin.

4. After completing the treatment, gradually reduce the energy **Level** to the minimum setting and press **Pause** to stop output. Remove the glass tube from the treatment area.

Effects of Direct Electrotherapy

1. Provides gentle warmth and vibration for a calming and smoothing effect on the skin.
2. Promotes blood circulation, helping to nourish the skin and improve radiance.
3. Enhances cellular metabolism, supporting natural skin functions.
4. Increases skin permeability, improving product absorption and overall skincare effectiveness.

Indirect Electrotherapy

1. Instruct the customer to hold the straight electrotherapy tube, then press the Start button to begin operation.
2. Gradually adjust the energy Level to the desired intensity while massaging the treatment area. Do not touch the electrodes during operation.
3. Before removing the glass electrode from the customer's hand, press the Pause button to stop output

Effects of Indirect Electrotherapy

- Stimulates blood circulation and enhances metabolism.
- Improves the skin's absorption of nutrients and resistance to bacteria.
- Enhances cellular vitality, improving the effectiveness of the treatment.

Specifications

Product Name:	High-Frequency Table Top Facial Unit HF
Voltage:	AC100-120V/220-240V
Frequency:	50/60Hz
Power Consumption:	20W
Dimensions(L*W*H):	12.0x10.0x8.9 inches
Net Weight:	4.6lbs

Warranty Information

The manufacturer (the “warrantor”) warrants to the original purchaser that this equipment will be free from defects under normal and proper operation for a period of one (1) year from the date of purchase. This warranty covers all parts and labor for that one (1) year period. This warranty shall not apply to any equipment that has been subjected to abuse, misuse and alteration of any type or to any defect or damage caused by repair, replacement, substitution, or use with parts other than parts approved by the manufacturer. The manufacturer shall not be liable for the loss of use of this equipment, loss of time or business, inconvenience or any other indirect, consequential, special or incidental damages due to defects covered by this warranty or any implied warranty. To implement this warranty, contact the dealer from whom you purchased the equipment. If necessary, you will be asked to return all, or the appropriate part, of the equipment. If warranted, the repairs will be performed at no charge and the equipment returned to you. Unit owner must prepay all shipping costs when returning items for warranty service. This limited warranty is the only written or express warranty given by the manufacturer. This warranty gives you specific legal rights but you may also have other rights, which may vary from state to state or province to province.

SKIN+ACT

Phone: 1-800-418-0830
Email: info@skinact.com
Website: skinact.com