
SKIN+ACT

Kye Electric Treatment Chair

PRODUCT MANUAL

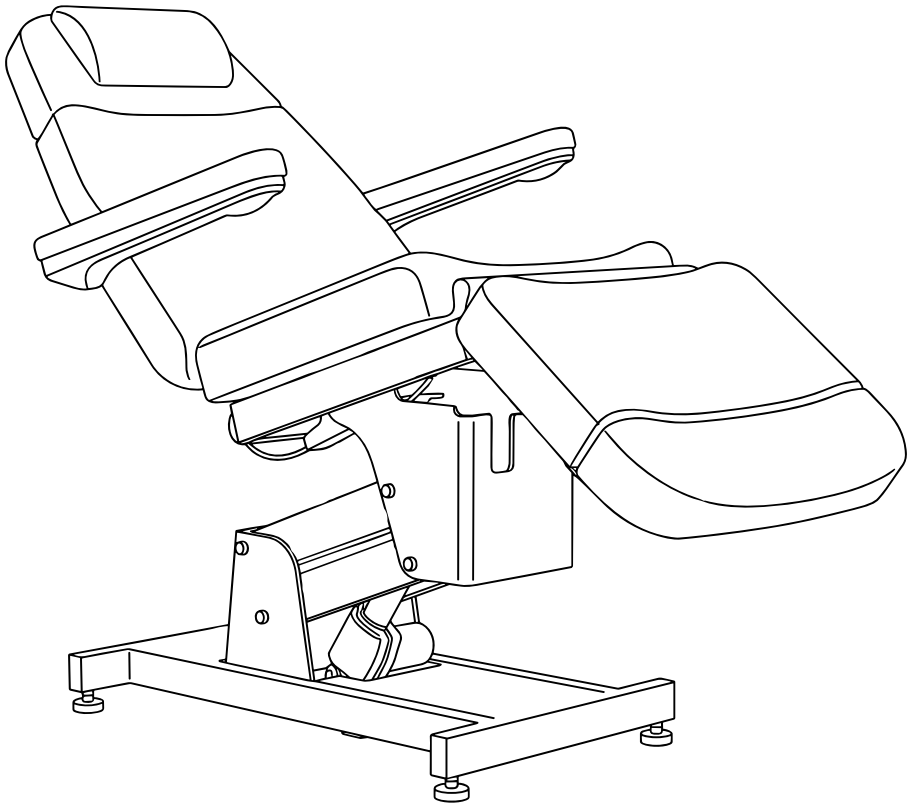

SKU26123

SKINACT.COM

TABLE OF CONTENTS

Notice & Disclaimer 3
Warnings 4
Safety and Maintenance Guidelines 5
Operating Guidelines 5
Stability and Rotation Safety 6
Installation 7
Structure of the Treatment Table 7
Dimensions and Angle Specifications 8
Remote Control Instructions 9
Cleaning and Maintenance 10
Circuit System Connection Diagram 10
Troubleshooting 11
Symbols & Safety Labels 12
Specifications 13
Warranty Information 14

NOTICE

No part of this document may be photocopied, reproduced, or translated into any other language without prior written consent of Spa and Equipment/SkinAct.
The information in this document is subject to change without notice at any time and should not be construed as a commitment by Spa and Equipment/SkinAct.
Spa and Equipment/SkinAct assumes no responsibility for any errors that may be in this document, nor does it make any express or implied warranty with regard to this material, including, but not limited to, the implied warranties of merchantability and fitness for a particular purpose.
Spa and Equipment/SkinAct shall not be liable for incidental or consequential damages arising out of the furnishing, performance, or use of this document and the program material which it describes.

DISCLAIMER

This product is intended for professional use by trained spa, salon, esthetic, wellness, or other qualified professionals. It must be used only for its intended purpose and in accordance with all instructions, warnings, contraindications, maintenance requirements, and safety guidelines provided in this manual.
The information in this manual is for general product operation and safety reference only. It does not replace professional training, licensing requirements, medical advice, service instructions, applicable laws, or workplace safety rules. Users are responsible for proper training, safe operation, inspection, client screening when applicable, sanitation, maintenance, and compliance with all applicable regulations.
SkinAct/Spa and Equipment does not provide medical advice and does not diagnose, treat, cure, or prevent any disease, medical condition, injury, or skin disorder. Any treatment descriptions, suggested uses, or expected results are for general cosmetic and professional use reference only, and results may vary.
Before each use, inspect the product, power cord, accessories, attachments, moving parts, and related components, as applicable, for damage, looseness, contamination, instability, or abnormal operation. Do not use the product if it appears damaged, defective, improperly assembled, unsafe, or if any component is missing or malfunctioning.
The user assumes full responsibility for proper assembly, installation, operation, client selection when applicable, treatment technique when applicable, cleaning, maintenance, and storage. SkinAct/Spa and Equipment shall not be responsible for injury, property damage, treatment complications, equipment damage, loss of business, or other damages resulting from misuse, improper use, lack of training, failure to follow instructions, unauthorized repairs or modifications, improper maintenance, or use outside the intended purpose.
Do not modify, disassemble, repair, or alter this product unless authorized in writing by SkinAct/Spa and Equipment or performed by an approved service provider. Unauthorized modification, misuse, improper maintenance, or failure to follow this manual may void the warranty.
Product designs, specifications, components, accessories, images, and instructions may vary from the actual product and may be changed or updated without prior notice.
This product contains electric adjustment components and moving parts. Improper use may cause injury, pinching, equipment damage, or unsafe operation. Users are responsible for operating the table safely and following all instructions, warnings, and maintenance requirements in this manual. The user is solely responsible for confirming that use of this device is permitted under applicable state/local laws, scope-of-practice rules, licensing requirements, and workplace safety standards. This device is not intended for self-use, home use, or use by untrained individuals.

Warnings

- Disconnect the power supply before replacing electrical components or performing maintenance or cleaning.
- Connect the power cord only to a properly installed and grounded electrical outlet to reduce the risk of fire and electric shock.
- Do not stand on the equipment.
- Keep this equipment out of the reach of children. Do not allow children to play with or operate the equipment. When leaving the equipment unattended, raise the backrest to its highest position.
- Do not use or store the equipment in wet or damp environments, such as bathrooms, as this may result in electric shock or equipment failure. Keep the hand controller and foot controller away from water.
- Do not operate the equipment near flammable paints, coatings, gases, or in oxygen-enriched environments.
- This equipment is not intended for use by persons (including children) with reduced physical, sensory, or mental capabilities, or by individuals lacking sufficient experience or knowledge, unless they are supervised or instructed by a person responsible for their safety.
- If the power cord is damaged, discontinue use immediately and contact SkinAct, an authorized service center, or a qualified service technician for repair or replacement.
- Before operating the chair, ensure that no objects or body parts are within the range of movement of any moving components.
- This equipment must be operated only by trained professionals.
- Do not service or perform maintenance on the equipment while it is in use by a patient.
- Do not use portable RF (radio frequency) transmitters or other electromagnetic transmitting devices near this equipment.
- Position the equipment so that the power cord remains easily accessible at all times.
- The third conductor in the power cord is the protective grounding conductor and must not be removed or modified.
- Maximum patient weight: 440 lb (200 kg). Exceeding this weight limit may result in equipment damage or personal injury.
- If the user or patient becomes aware of a serious incident involving this equipment, report it to the appropriate regulatory authority and to SkinAct as soon as possible.
- Dispose of the equipment and its accessories in accordance with applicable local regulations at the end of their service life.
- Do not modify this equipment. Unauthorized modifications may affect safety and performance.
- This equipment is intended for operation by licensed medical or aesthetic professionals. Patients should not operate the equipment themselves.
- The patient should remain aware of their surroundings during treatment and should always be supervised by the operator.
- This product is upholstered with artificial leather. If you experience an allergic reaction to the upholstery material, discontinue use immediately.
- During operation, the surface temperature of the hand controller, button panel, and metal frame may reach 106°F (41°C) but will not exceed 113°F (45°C). Patients should not remain in contact with these surfaces for extended periods (contact time should be less than 1 minute).

Safety and Maintenance Guidelines

To ensure safe and proper operation of this electric treatment table, please read the following instructions carefully and retain this manual for future reference.

- Do not inspect, adjust, repair, or perform maintenance on the equipment while it is operating or occupied.
- Regularly inspect and tighten all bolts, nuts, and fasteners to help prevent loose components, instability, vibration, or falls.
- Do not operate the equipment if it is damaged or malfunctioning. If unusual movement, noise, odor, vibration, or another abnormal condition occurs, stop operation immediately and disconnect the power. Resume use only after the problem has been corrected.
- This equipment is not intended for use by children. Keep children away from the equipment and do not allow them to play with the controls.
- Individuals with reduced physical, sensory, or cognitive abilities, or insufficient training and experience may use the equipment only under appropriate supervision.
- After each client, clean the upholstery with a soft cloth lightly dampened with a mild soap-and-water solution. Do not use abrasive cleaners, harsh chemicals, or excessive moisture.
- Maintenance and repairs must be performed only by qualified service personnel authorized by SkinAct.
- Keep remote controls and hand controls away from children and store them securely when not in use.
- If the equipment causes or contributes to a serious injury or other serious incident, discontinue use and report the incident to SkinAct and the appropriate regulatory authority when required.

Operating Guidelines

- Read this manual completely before installation, operation, or adjustment. Keep it in a safe location for future reference.
- Inspect the table before each use. Confirm that all components, safety features, cables, and controls are properly installed and in good working condition.
- Do not exceed the table's maximum weight capacity.
- Operate the table only under safe conditions and on a stable, level surface.
- Before adjusting the table, make sure the client and operator are positioned safely and all body parts, clothing, cords, and nearby objects are clear of moving components and pinch points.
- Table movements are controlled by hold-to-operate buttons. Press and hold the appropriate button until the desired position is reached, then release it to stop movement.
- Avoid placing concentrated weight or pressure on one area of the table. Distribute the client's weight evenly across the surface.
- Motor duty cycle: Operate the motor for no more than 2 continuous minutes, followed by at least 18 minutes of rest.
- Keep hands, feet, hair, clothing, and other body parts away from moving components and the pinch points identified in this manual.

Stability and Rotation Safety


When operating a hydraulic rotating chair or single-post electric treatment table, the operator is responsible for maintaining stability and ensuring client safety. Always follow the instructions provided for the specific model.

To Ensure Stability

1. Place the chair or table on a level, dry, and non-slip surface. Adjust the leveling feet, if equipped, so the base remains stable and does not rock.
2. Inspect the base, controls, adjustment mechanisms, and fasteners before each use. Do not operate the unit if any component is loose, damaged, or functioning improperly.
3. Keep the client's weight centered over the base. Position the chair or tabletop in line with the base whenever possible, particularly during treatment.
4. Do not allow anyone to sit, stand, lean, or place excessive weight on the headrest, backrest, leg rest, foot section, or armrests.
5. Whenever possible, rotate or reposition the unit before the client is seated or positioned on it. Do not rotate or adjust the unit while the client is entering or exiting.
6. If rotation is necessary while occupied, place the client in a stable upright position, keep the client centered, support the chair or table securely, and rotate it slowly.
7. Keep hands, feet, clothing, cords, and other objects away from moving parts and potential pinch points during rotation or adjustment.
8. Ensure all rotation locks and adjustable sections are securely engaged before beginning treatment.
9. Do not exceed the stated weight capacity or apply sudden, concentrated, or excessive downward pressure. These products are not intended for massage or procedures that require substantial downward force.
10. Do not leave a client unattended while the unit is elevated, reclined, rotating, or being adjusted.
11. Stop using the unit immediately if it becomes unstable, shifts unexpectedly, makes unusual sounds, or fails to hold its selected position.




Warning: Do Not Sit or Apply Excess Force
Do not sit, stand, jump, or place excessive weight on the backrest or footrest. Doing so may cause the product to tip, damage the backrest or footrest joints, or result in injury.




Recommended Maximum Load Distribution

Installation

1. Unpack the table and inspect it for damage. Confirm that all accessories, hardware, and components are included. If any item is missing or damaged, do not use the table and contact SkinAct.
2. Place the table in a clean, dry treatment area with sufficient clearance around all sides for safe operation and adjustment.
3. Position the table on a stable, level, nonslip floor.
4. If the table is uneven, rotate the adjustable leveling feet until the table is level and stable.
5. No additional screws or floor anchors are required to secure the table to the floor.
6. Connect the power cord to the table, then plug it into a properly grounded electrical outlet that matches the electrical rating on the product label.
7. Arrange nearby furniture and equipment so they do not interfere with the table's movement or create crushing, pinching, entrapment, or tripping hazards.
8. Before use, operate each adjustment through its full range without a client on the table to confirm that the table moves correctly and has sufficient clearance.

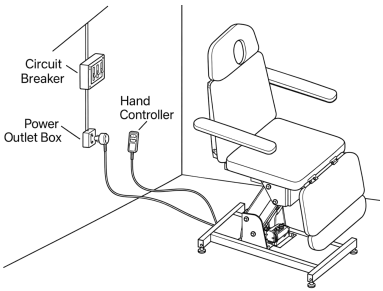

Structure of the Treatment Table

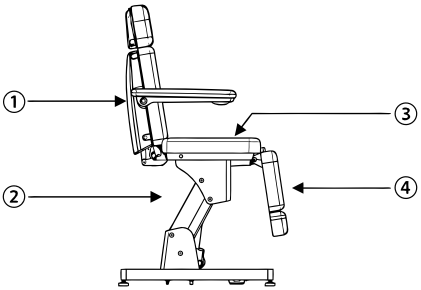

① Backrest Angle Adjustment


② Height Adjustment


③ Seat-Tilt Adjustment

④ Leg-Rest Angle Adjustment

Important: Keep hands, feet, the head, and other body parts away from moving components and pinch points during adjustment.


Dimensions and Angle Specifications

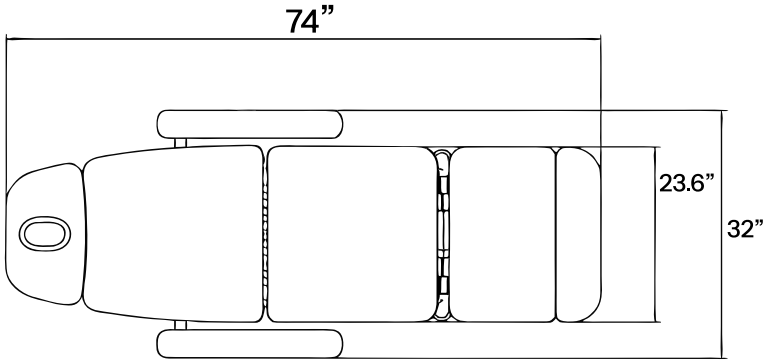

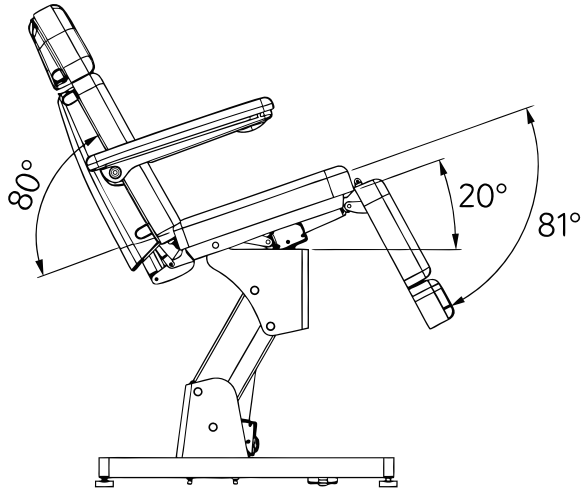

Dimensional tolerances range from ±0.25 to ±1.2 inches.

Remote Control Instructions

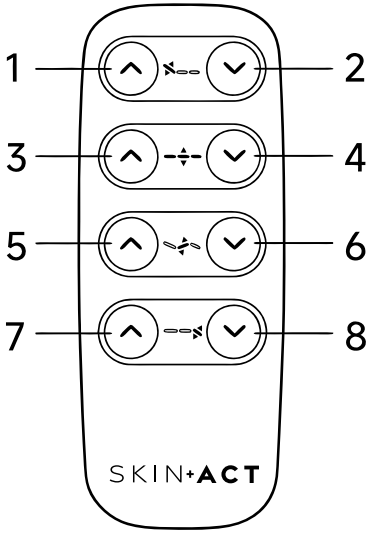


No.	Function
1/2	Backrest Adjustment — Up or Down
3/4	Height Adjustment — Up or Down
5/6	Seat-Tilt Adjustment — Up or Down
7/8	Leg-Rest Adjustment — Up or Down

Cleaning and Maintenance

- When cleaning and sanitizing, do not use bleach, Barbicide, or other harsh chemicals. Using harsh chemicals can damage the upholstery.
- For best results, clean with **SkinAct All-In-One Upholstery & Disinfecting Multi-Purpose Cleaner** (SKU24261).
- Clean and sanitize the upholstery after each treatment.
- Lubricate only manufacturer-approved hinge and pivot points using a compatible lubricant. Do not apply lubricant to motors, electrical components, upholstery, or control mechanisms.
- If the headrest mechanism becomes difficult to adjust, discontinue use and contact SkinAct for assistance.
- Every six months, visually inspect all visible parts of the unit. If there are any abnormal noises or vibrations during operation, call Spa & Equipment/SkinAct at 1-800-418-0830.

Circuit System Connection Diagram

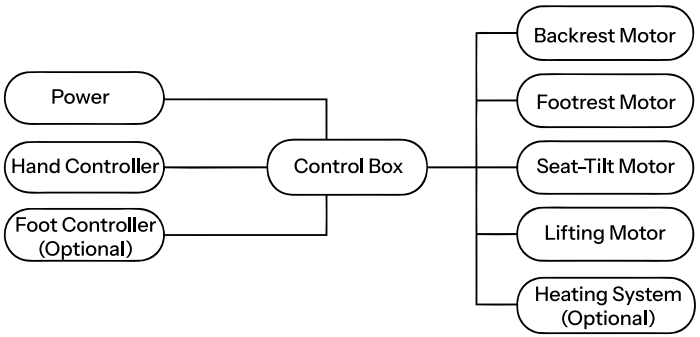

⚠ The maximum weight capacity of the chair is 440 lb (200 kg). Exceeding this limit may result in equipment damage or personal injury.

Troubleshooting

Motorized Sections Do Not Move

Solution: Confirm that the hand or foot remote is securely connected and responding properly. If the remote does not respond, replace the remote or contact SkinAct/Spa & Equipment technical support for assistance.

Hand or Foot Remote Not Working

Solution: Check that the remote is securely connected. If it remains unresponsive, replace the controller or contact SkinAct/Spa & Equipment.

Control Box or Motor Connection Issue

Solution: If the motorized sections do not move after confirming the remote and power connection, discontinue use and contact Spa & Equipment/SkinAct.

Abnormal Noise During Operation

Solution: Stop using the product. Lubricate only accessible, manufacturer-approved hinge and pivot points using a compatible lubricant, as directed in the Cleaning and Maintenance section. Do not apply lubricant to motors, electrical components, internal lift mechanisms, upholstery, or controls. If the noise continues, contact SkinAct/Spa & Equipment.

Motor Performance Issue

Solution: If the motor moves unevenly, produces unusual noise, stops unexpectedly, or fails to operate smoothly, discontinue use and contact SkinAct. The motor may require inspection or replacement by a qualified service technician.

Do not open the control box, motor, or electrical housing. If the problem continues after completing the steps above, unplug the table and contact SkinAct.

 Refer to instruction manual	 Manufacturer
 WEEE	 CE
 Date of Manufacture	EU REP Authorized representative in the European Community
 Warning	SN Serial No.
 Keep dry / Protect from Rain	 Fragile, handle with care
 Keep away from sunlight	 Maximum Stacking Load: 250 kg
 This Side Up	 Do Not Roll or Tumble
 Handle with Care	 Do Not Clamp
UK CA UK Conformity Assessed	

Specifications

Product Name:	Kye Electric Treatment Chair
Voltage:	100–120 V AC
Frequency:	50/60 Hz
Power Consumption:	300 W
Leg-Rest Adjustment:	Up to 81°
Backrest Adjustment:	0° (flat) to 80° (inclined)
Seat-Tilt Adjustment:	Up to 20°
Length:	74”
Width:	32”
Width without armrests:	23.6”
Relative Humidity:	30%–90%
Weight Capacity:	440 lb (200 kg)
Operating Temperature:	32°F–104°F (0°C–40°C)

Warranty Information

The manufacturer/warrantor warrants to the original purchaser that this product will be free from defects in materials and workmanship under normal and proper use for a period of one (1) year from the original date of purchase, unless otherwise stated in writing for a specific product.

This limited warranty applies only to the original purchaser and is not transferable. Proof of purchase may be required to obtain warranty service.

This warranty covers parts and labor required to correct defects in materials or workmanship during the warranty period. At the warrantor's discretion, the product may be repaired, replaced, or substituted with a comparable item or component.

This warranty does not cover damage or defects caused by misuse, abuse, improper assembly, improper installation, unauthorized modification, unauthorized repair, neglect, accident, improper cleaning, use of harsh chemicals, power surges, water or liquid damage, use outside the intended purpose, failure to follow the product manual, or use with parts/accessories not approved by SkinAct.

This warranty does not cover normal wear and tear, cosmetic damage, upholstery wear, stains, discoloration, scratches, dents, wheels/casters, bulbs, glass parts, filters, tips, probes, disposable parts, consumables, or accessories subject to regular replacement unless the defect is determined to be due to a manufacturing issue.

The warrantor shall not be liable for loss of use, loss of time, loss of business, lost revenue, inconvenience, or any indirect, incidental, special, or consequential damages arising from the use of this product or from any defect covered by this warranty.

To request warranty service, contact the dealer or SkinAct customer support. If return service is required, the purchaser may be asked to return the product or the affected component for inspection. The purchaser is responsible for properly packaging the item and prepaying all shipping costs to send the item in for warranty service. If the issue is covered under warranty, repair or replacement will be performed at no charge, subject to the terms of this limited warranty.

The warranty does not cover damage, contamination, upholstery damage, sanitation-related issues, injury claims, or equipment issues resulting from improper cleaning, improper maintenance, misuse, use by untrained users, or use outside applicable safety guidelines.

This limited warranty is the only written or express warranty provided by the warrantor. No employee, representative, dealer, or third party is authorized to modify or extend this warranty unless confirmed in writing by SkinAct. This warranty gives you specific legal rights, and you may also have other rights, which vary by state or province.

SKIN+ACT

Phone: 1-800-418-0830

Email: info@skinact.com

Website: www.skinact.com